


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121819\
Data File : BN009019.D
Acq On : 18 Dec 2019 14:25
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN120919.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 19 00:50:46 2019

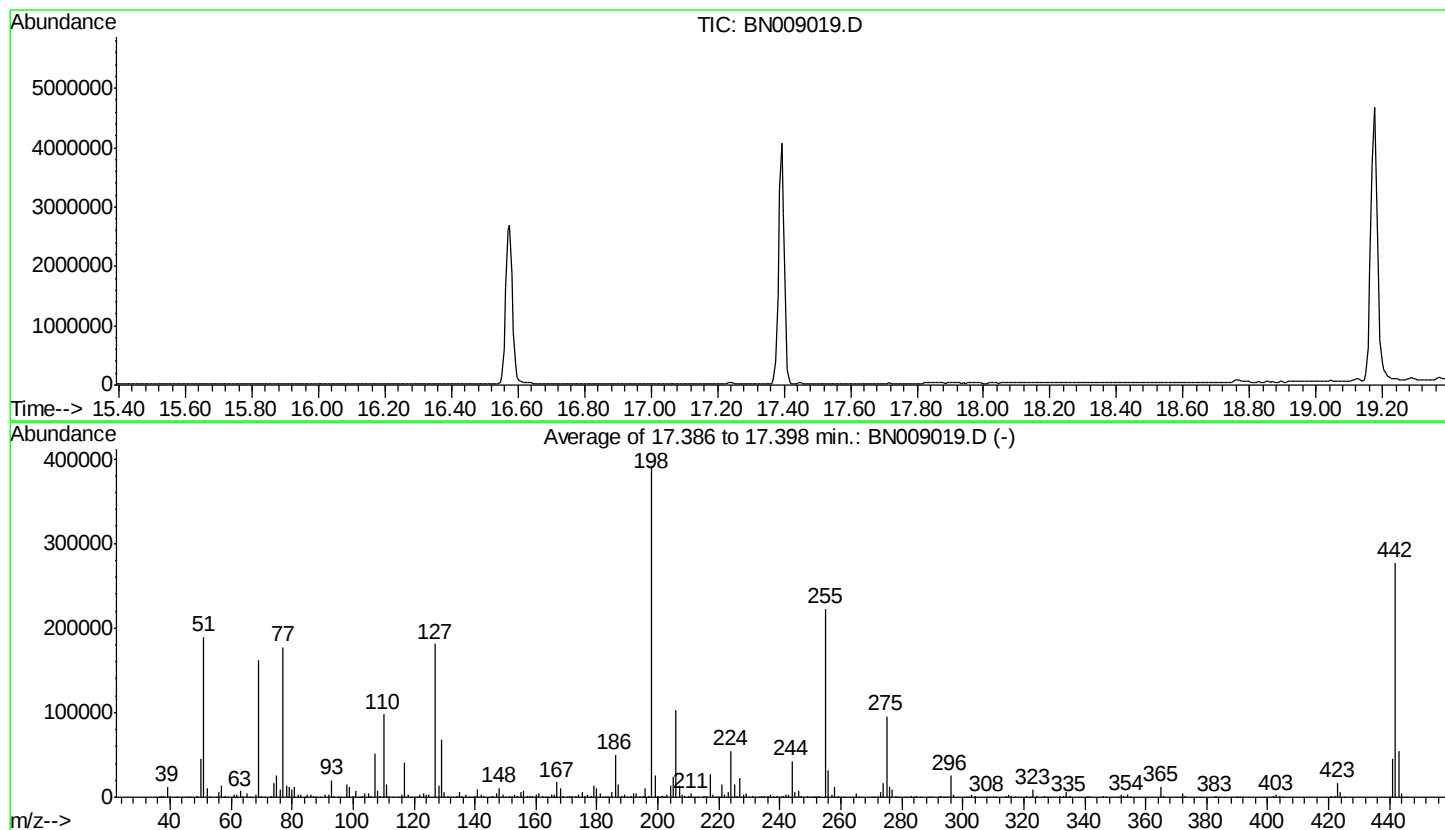

AutoFind: Scans 2448, 2449, 2450; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.4	189597	PASS
68	69	0.00	2	1.9	3074	PASS
69	198	0.00	100	41.5	162464	PASS
70	69	0.00	2	0.5	882	PASS
127	198	10	80	46.2	181098	PASS
197	198	0.00	2	0.3	1277	PASS
198	198	100	100	100.0	391850	PASS
199	198	5	9	6.6	25909	PASS
275	198	10	60	24.3	95408	PASS
365	198	1	100	3.2	12362	PASS
441	198	0.01	100	11.7	45680	PASS
442	198	50	100	70.7	276885	PASS
443	442	15	24	19.5	53938	PASS