
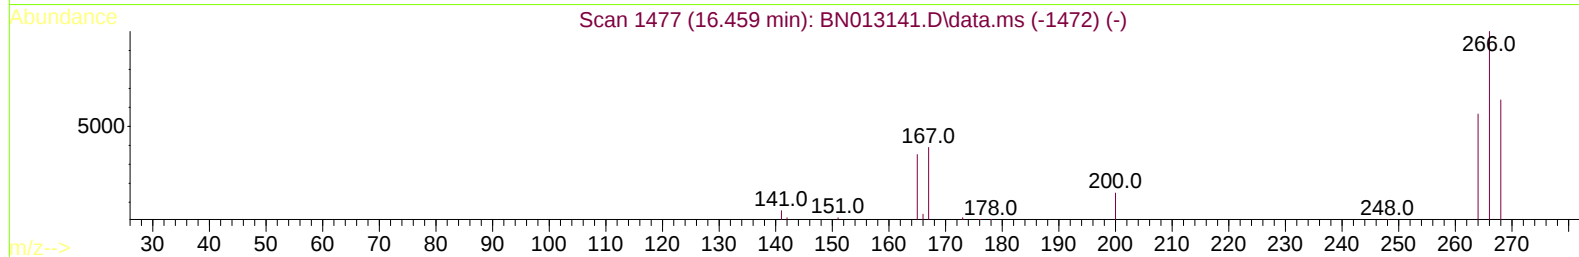
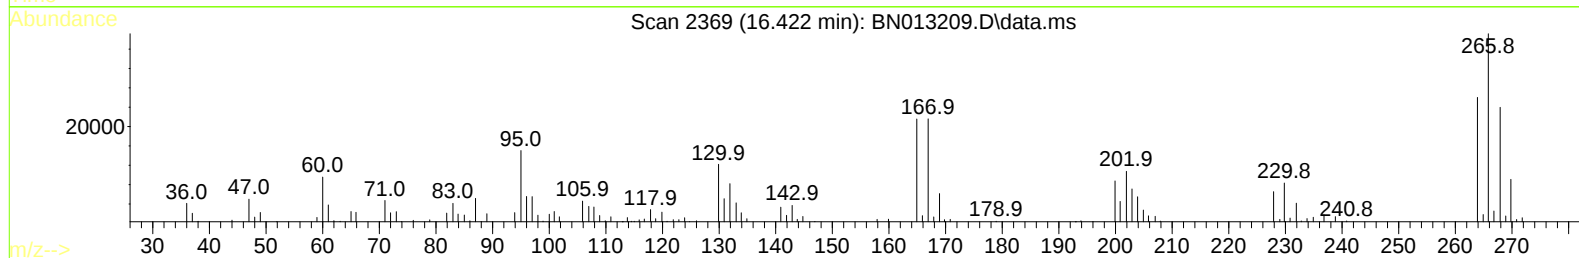


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121820\
 Data File : BN013209.D
 Acq On : 18 Dec 2020 14:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 03:30:01 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 18 16:11:20 2020
 Response via : Initial Calibration

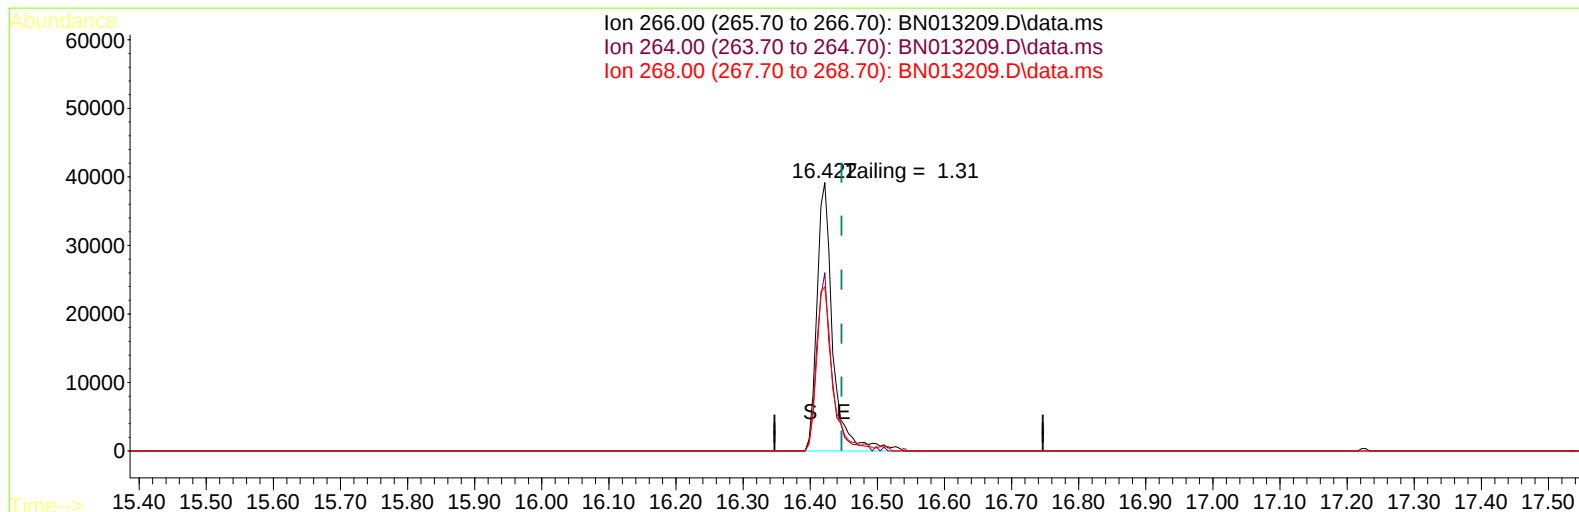

TIC: BN013209.D\data.ms

(24) Pentachlorophenol

16.422min (-0.025) 0.00 ng

response 64243

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	63.60	62.43
268.00	64.40	62.58
0.00	0.00	0.00