

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121820\
 Data File : BN013216.D
 Acq On : 18 Dec 2020 19:41
 Operator : CG/JU
 Sample : L5124-16
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BPOW1-8-20201215

Quant Time: Dec 19 01:11:43 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 18 16:11:20 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.338	152	588	0.40	ng	0.00
7) Naphthalene-d8	10.125	136	1546	0.40	ng	# 0.01
13) Acenaphthene-d10	14.004	164	1013	0.40	ng	0.00
19) Phenanthrene-d10	16.775	188	2298	0.40	ng	# 0.00
29) Chrysene-d12	21.003	240	2672	0.40	ng	# 0.00
36) Perylene-d12	23.089	264	2933	0.40	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	4.970	112	206	0.09	ng	0.00
5) Phenol-d6	6.549	99	117	0.05	ng	0.00
8) Nitrobenzene-d5	8.553	82	335	0.21	ng	0.03
11) 2-Methylnaphthalene-d10	11.733	152	623	0.23	ng	0.00
14) 2,4,6-Tribromophenol	15.539	330	146	0.23	ng	0.00
15) 2-Fluorobiphenyl	12.621	172	997	0.23	ng	-0.01
27) Fluoranthene-d10	18.823	212	2288	0.30	ng	0.00
31) Terphenyl-d14	19.434	244	1955	0.29	ng	-0.01


Target Compounds	Qvalue
-----	-----


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121820\
Data File : BN013216.D
Acq On : 18 Dec 2020 19:41
Operator : CG/JU
Sample : L5124-16
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BPOW1-8-20201215

Quant Time: Dec 19 01:11:43 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 18 16:11:20 2020
Response via : Initial Calibration




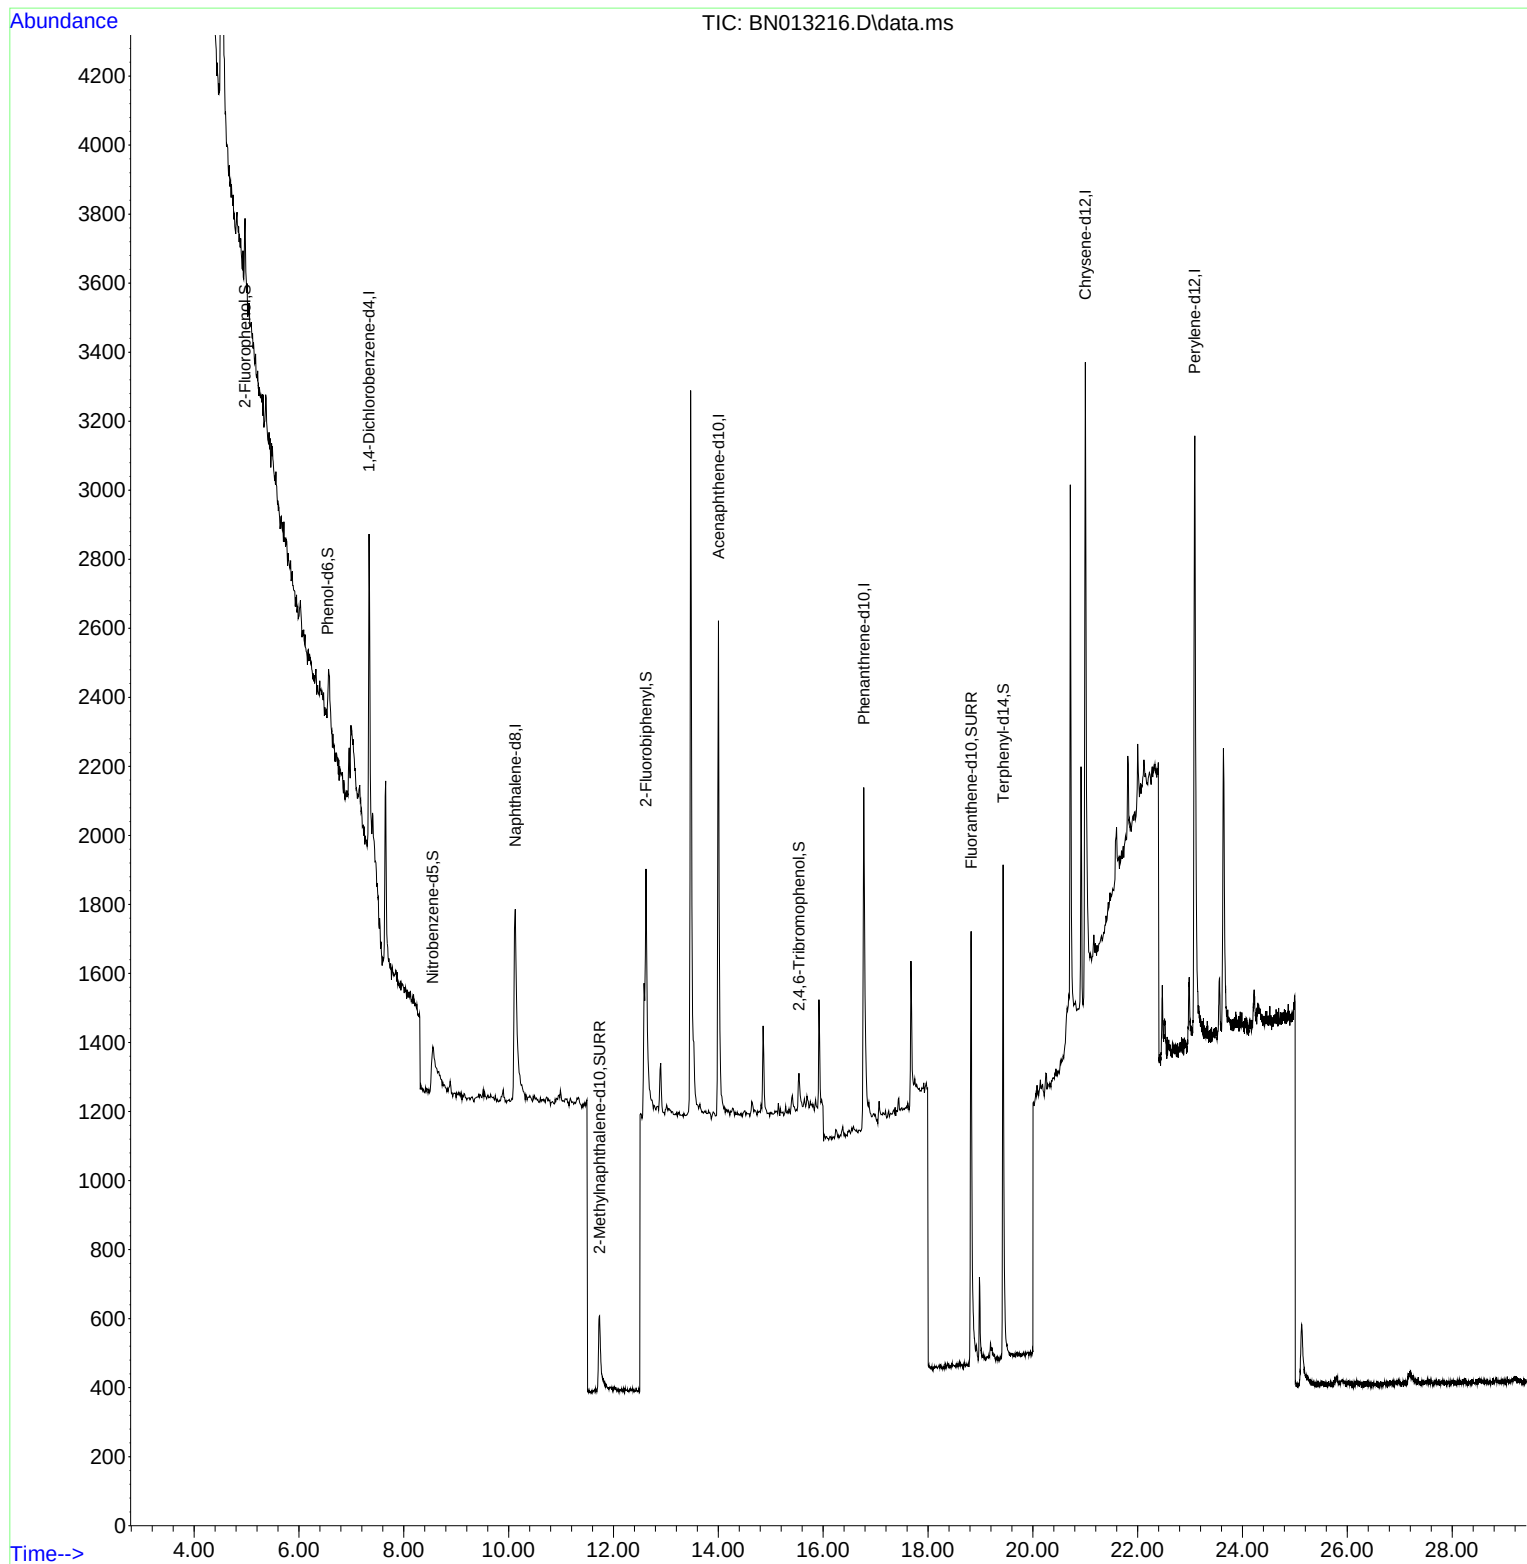


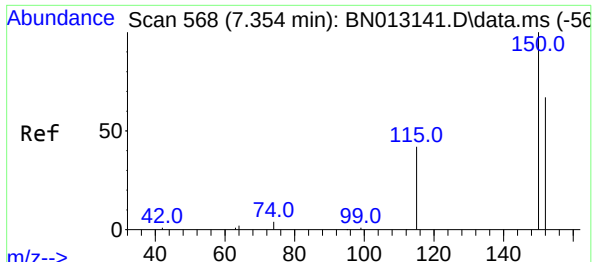

#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.338 min Scan# 566
Delta R.T. -0.008 min
Lab File: BN013216.D
Acq: 18 Dec 2020 19:41




Instrument :
BNA_N
ClientSampleId :
BPOW1-8-20201215


Tgt Ion:152 Resp: 588
Ion Ratio Lower Upper
152 100
150 144.0 116.6 174.8
115 73.2 52.9 79.3

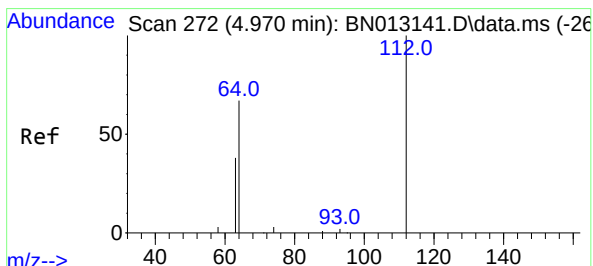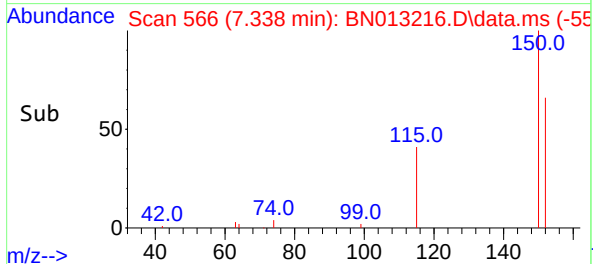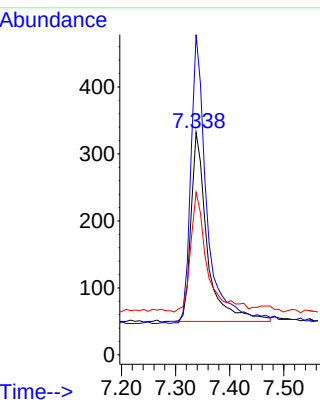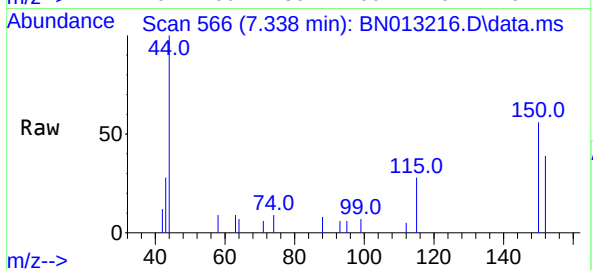

#4
2-Fluorophenol
Concen: 0.09 ng
RT: 4.970 min Scan# 272
Delta R.T. 0.008 min
Lab File: BN013216.D
Acq: 18 Dec 2020 19:41

Tgt Ion:112 Resp: 206
Ion Ratio Lower Upper
112 100
64 69.4 49.5 74.3
63 46.6 32.0 48.0

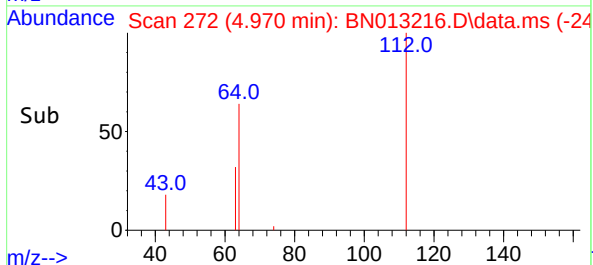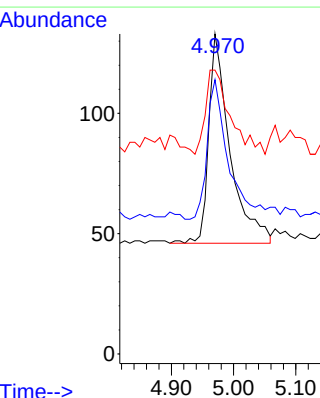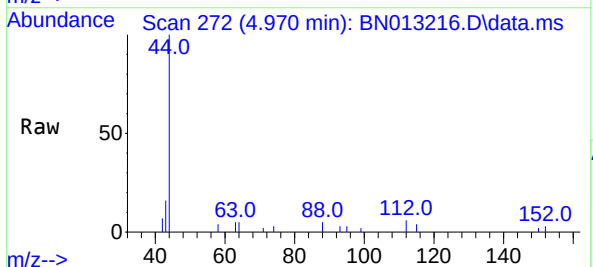




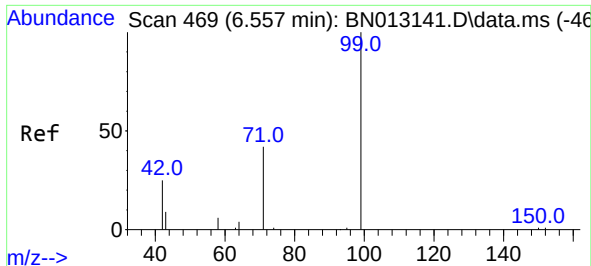


#5
Phenol-d6
Concen: 0.05 ng
RT: 6.549 min Scan# 468
Delta R.T. -0.000 min
Lab File: BN013216.D
Acq: 18 Dec 2020 19:41

Instrument :
BNA_N
ClientSampleId :
BPOW1-8-20201215

Tgt Ion: 99 Resp: 117




Ion	Ratio	Lower	Upper
99	100		
42	35.9	22.4	33.6#
71	41.9	37.8	56.6

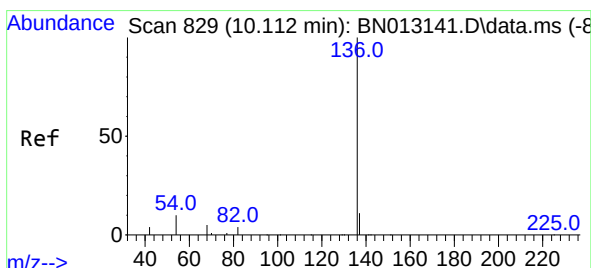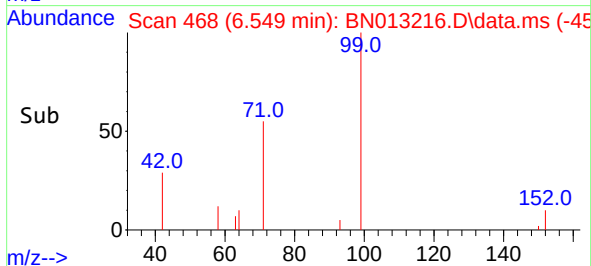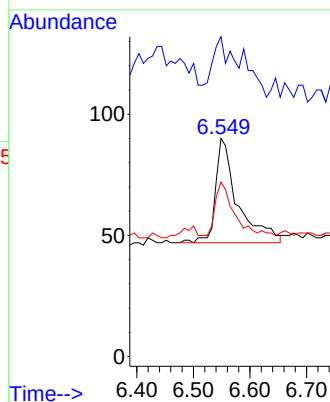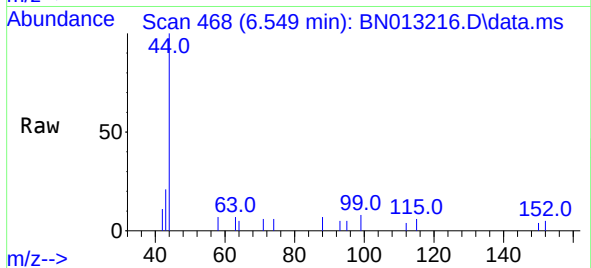


#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.125 min Scan# 830
Delta R.T. 0.013 min
Lab File: BN013216.D
Acq: 18 Dec 2020 19:41

Tgt Ion: 136 Resp: 1546

Ion	Ratio	Lower	Upper
136	100		
137	19.6	10.6	15.8#
54	18.7	8.6	12.8#
68	14.3	5.7	8.5#


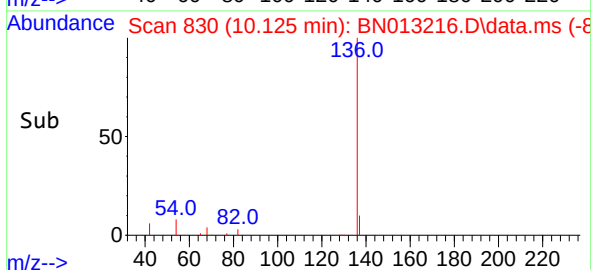
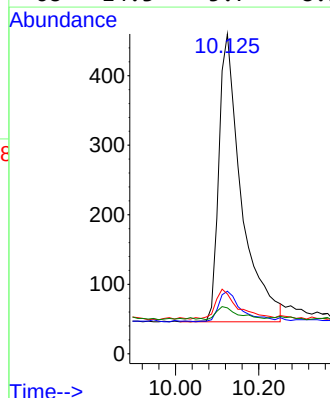
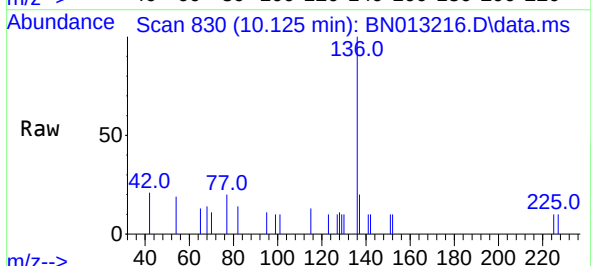


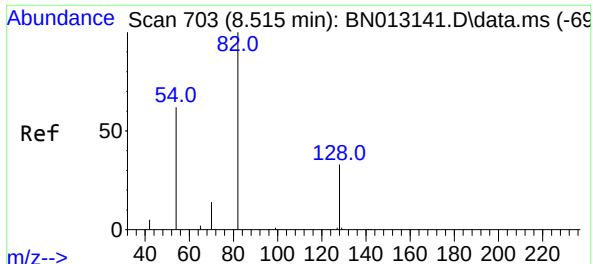

#8
Nitrobenzene-d5
Concen: 0.21 ng
RT: 8.553 min Scan# 706
Delta R.T. 0.025 min
Lab File: BN013216.D
Acq: 18 Dec 2020 19:41




Instrument :
BNA_N
ClientSampleId :
BPOW1-8-20201215


Tgt Ion: 82 Resp: 335
Ion Ratio Lower Upper
82 100
128 67.0 30.6 46.0#
54 83.0 48.3 72.5#

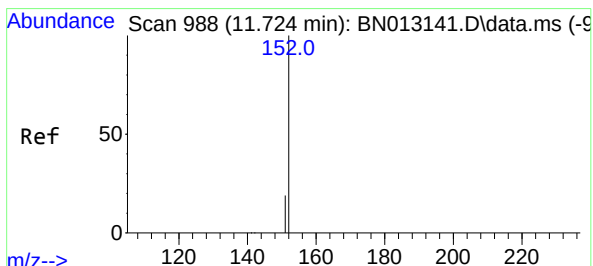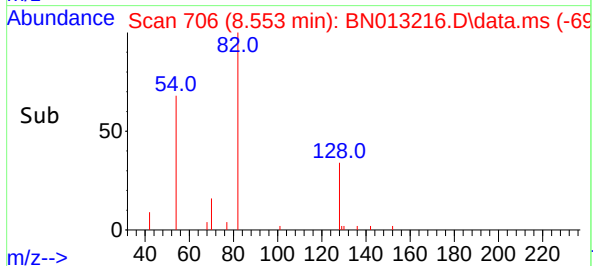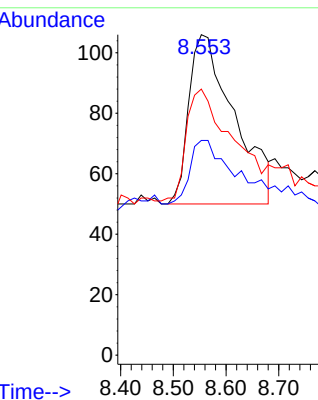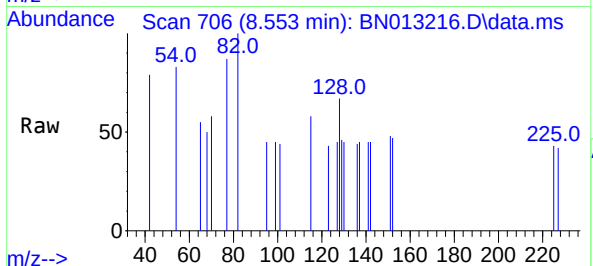

#11
2-Methylnaphthalene-d10
Concen: 0.23 ng
RT: 11.733 min Scan# 990
Delta R.T. 0.009 min
Lab File: BN013216.D
Acq: 18 Dec 2020 19:41

Tgt Ion: 152 Resp: 623
Ion Ratio Lower Upper
152 100
151 19.6 16.7 25.1


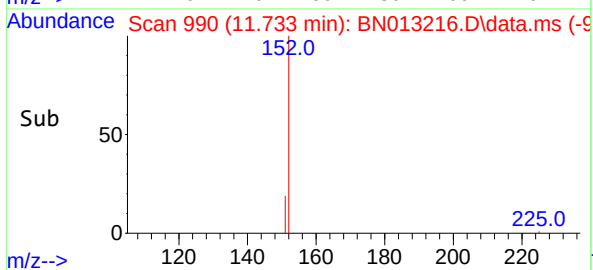
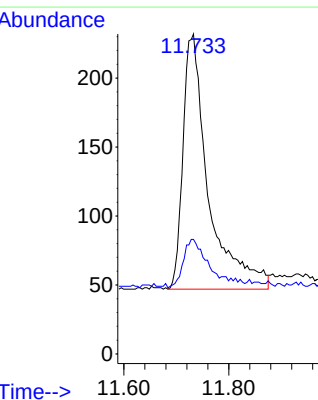
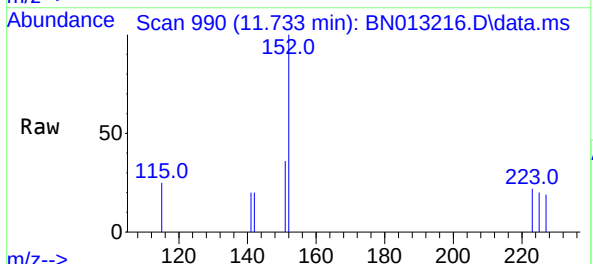


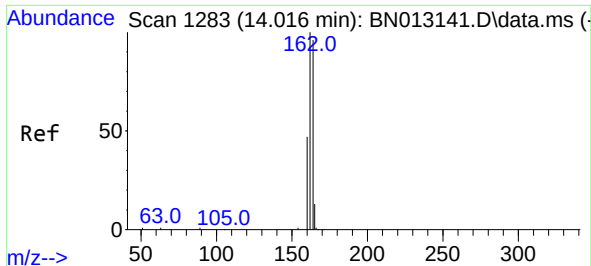

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.004 min Scan# 1282
Delta R.T. -0.000 min
Lab File: BN013216.D
Acq: 18 Dec 2020 19:41




Instrument :
BNA_N
ClientSampleId :
BPOW1-8-20201215


Tgt Ion:164 Resp: 1013
Ion Ratio Lower Upper
164 100
162 103.3 80.6 120.8
160 54.1 39.5 59.3

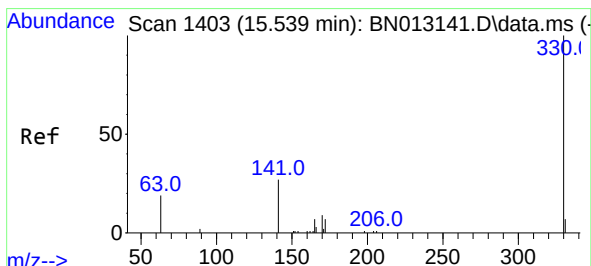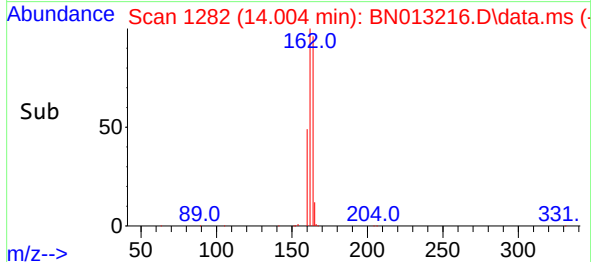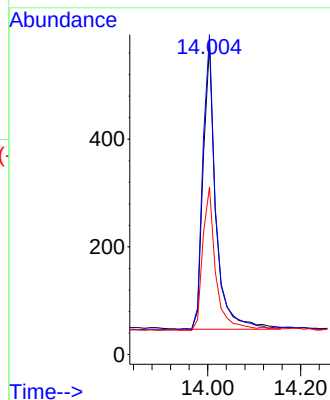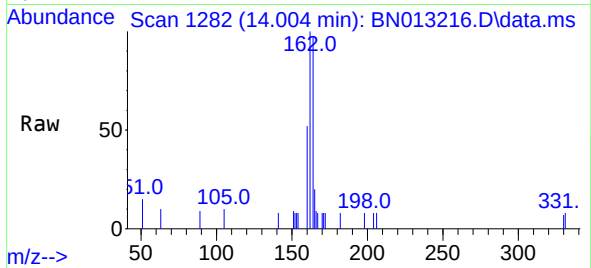

#14
2,4,6-Tribromophenol
Concen: 0.23 ng
RT: 15.539 min Scan# 1403
Delta R.T. -0.000 min
Lab File: BN013216.D
Acq: 18 Dec 2020 19:41

Tgt Ion:330 Resp: 146
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 57.5 34.4 51.6#


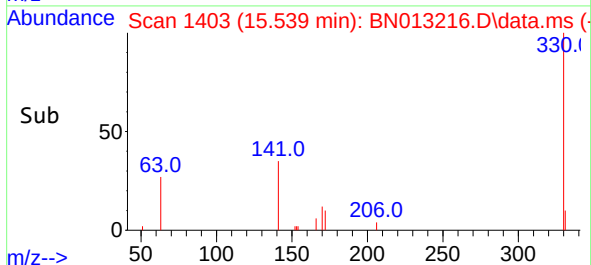
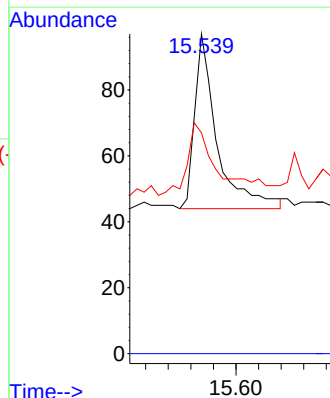
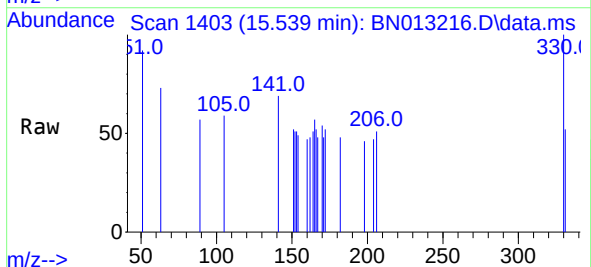


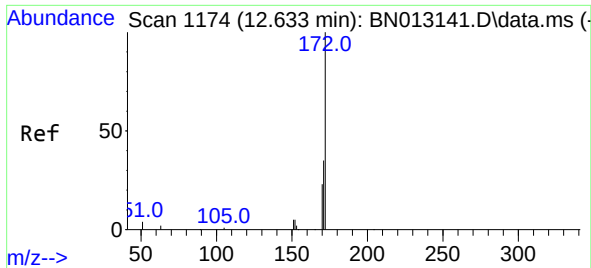

#15
2-Fluorobiphenyl
Concen: 0.23 ng
RT: 12.621 min Scan# 1173
Delta R.T. -0.013 min
Lab File: BN013216.D
Acq: 18 Dec 2020 19:41




Instrument :
BNA_N
ClientSampleId :
BPOW1-8-20201215


Tgt Ion:	172	Resp:	997
Ion	Ratio	Lower	Upper
172	100		
171	41.2	28.2	42.4
170	31.8	20.0	30.0#

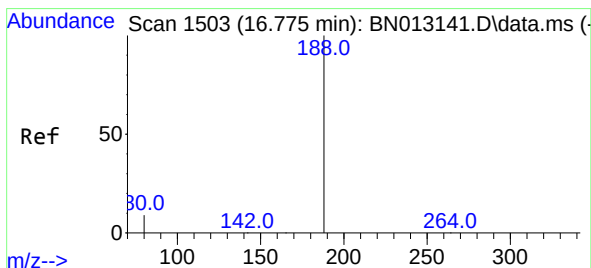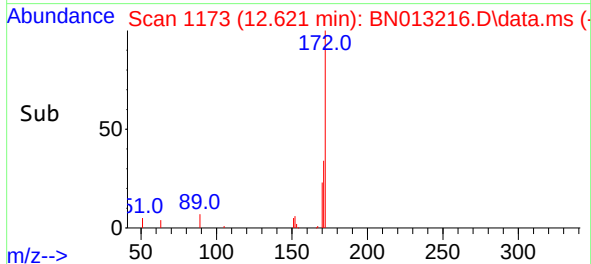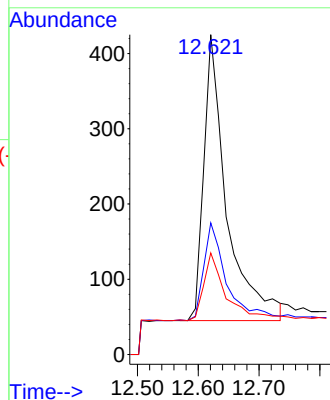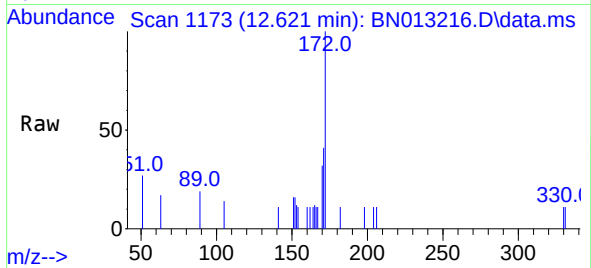

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 16.775 min Scan# 1503
Delta R.T. -0.001 min
Lab File: BN013216.D
Acq: 18 Dec 2020 19:41

Tgt Ion:	188	Resp:	2298
Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	12.5	5.0	7.4#


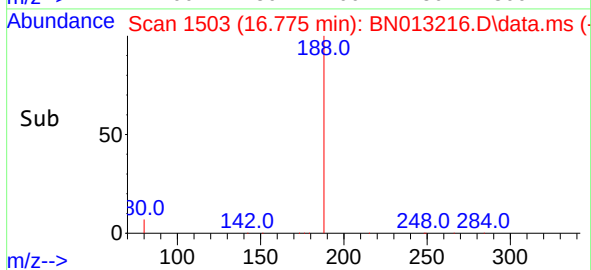
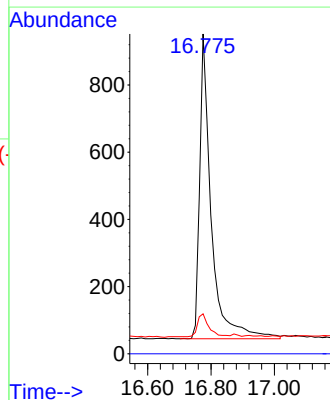
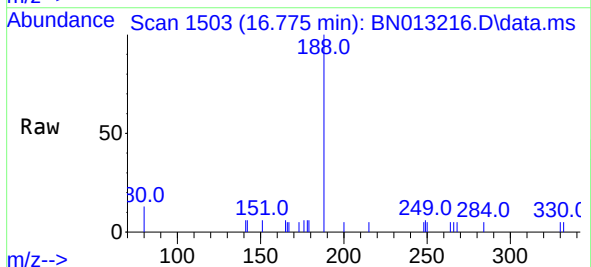


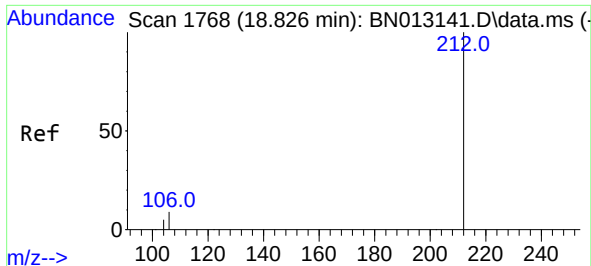

#27
Fluoranthene-d10
Concen: 0.30 ng
RT: 18.823 min Scan# 1769
Delta R.T. 0.002 min
Lab File: BN013216.D
Acq: 18 Dec 2020 19:41




Instrument :
BNA_N
ClientSampleId :
BPOW1-8-20201215


Tgt Ion:	212	Resp:	2288
Ion Ratio	Lower	Upper	
212	100		
106	8.2	6.8	10.2
104	4.3	4.1	6.1

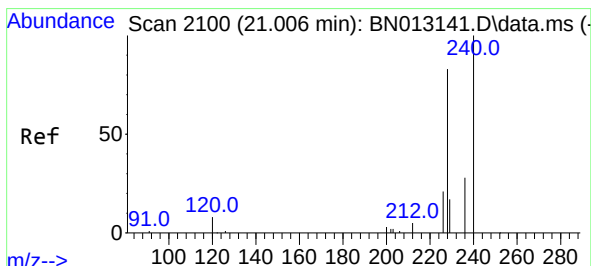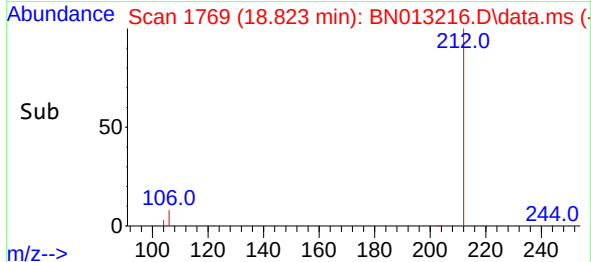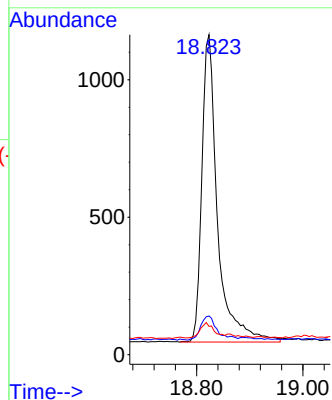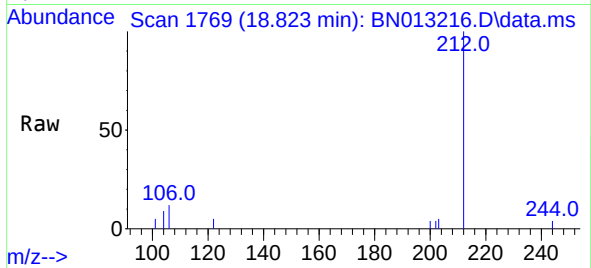

#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.003 min Scan# 2101
Delta R.T. -0.003 min
Lab File: BN013216.D
Acq: 18 Dec 2020 19:41

Tgt Ion:	240	Resp:	2672
Ion Ratio	Lower	Upper	
240	100		
120	12.4	5.3	7.9#
236	29.6	21.8	32.8

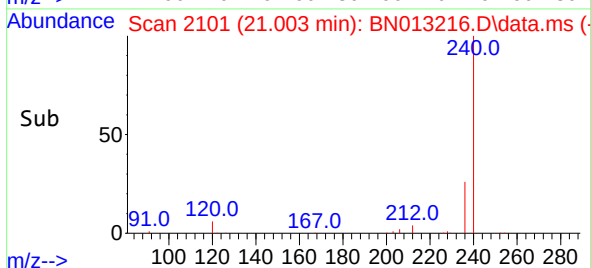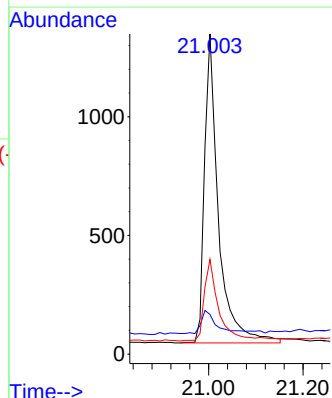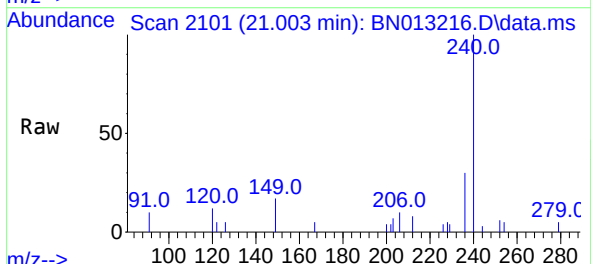




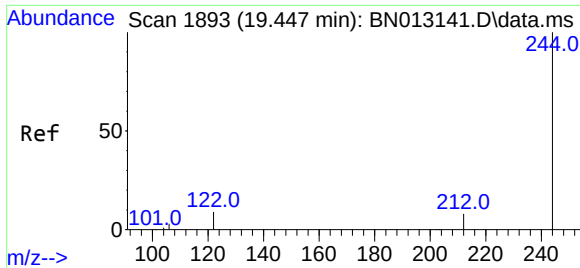


#31
Terphenyl-d14
Concen: 0.29 ng
RT: 19.434 min Scan# 1892
Delta R.T. -0.013 min
Lab File: BN013216.D
Acq: 18 Dec 2020 19:41

Instrument :
BNA_N
ClientSampleId :
BPOW1-8-20201215

Tgt Ion:244 Resp: 1955

Ion	Ratio	Lower	Upper
244	100		
212	12.9	7.3	10.9#
122	12.6	7.3	10.9#

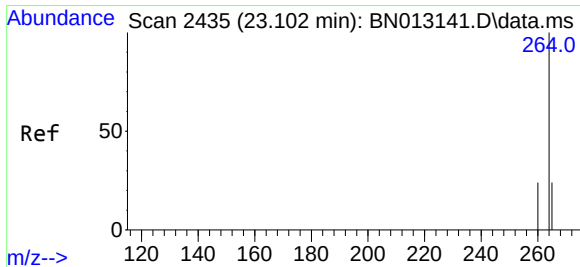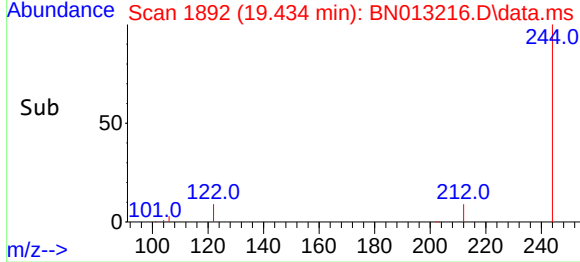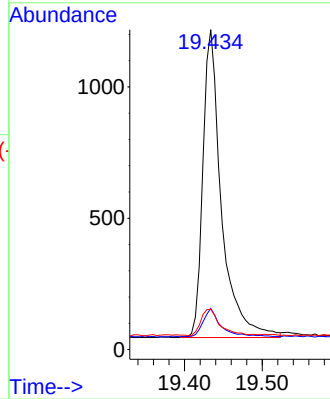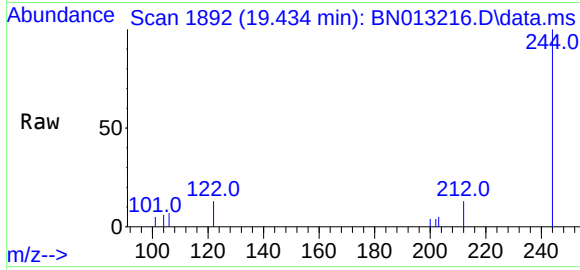

#36
Perylene-d12
Concen: 0.40 ng
RT: 23.089 min Scan# 2433
Delta R.T. -0.006 min
Lab File: BN013216.D
Acq: 18 Dec 2020 19:41

Tgt Ion:264 Resp: 2933

Ion	Ratio	Lower	Upper
264	100		
260	27.3	19.8	29.6
265	83.6	51.4	77.0#

