


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121820\
 Data File : BN013209.D
 Acq On : 18 Dec 2020 14:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 18 16:11:20 2020

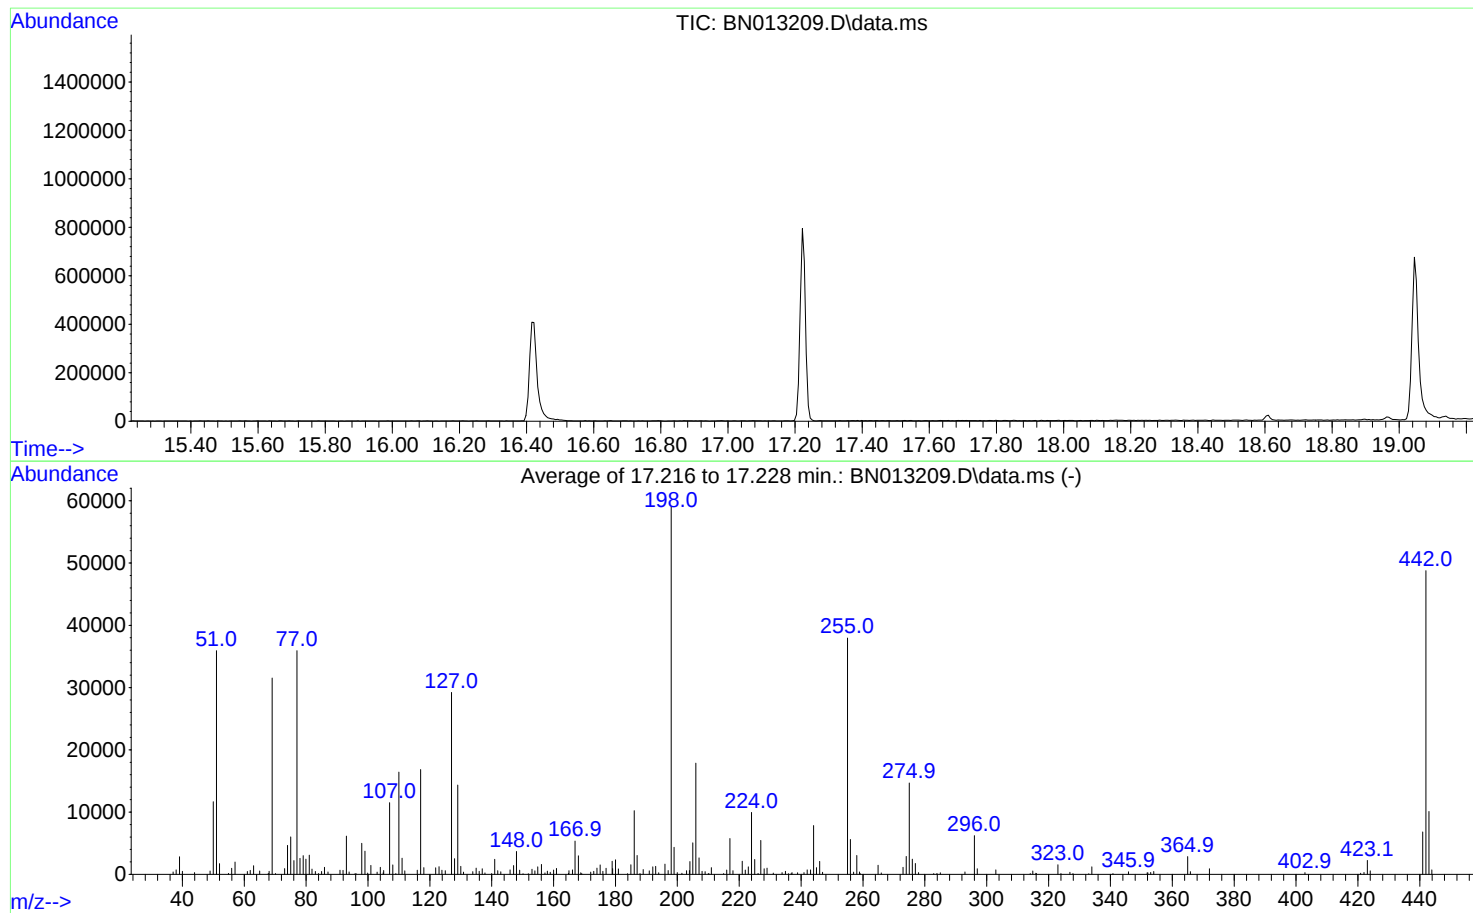

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.8	35931	PASS
68	69	0.00	2	1.5	486	PASS
69	198	0.00	100	53.4	31531	PASS
70	69	0.00	2	0.4	121	PASS
127	198	10	80	49.4	29208	PASS
197	198	0.00	2	1.0	614	PASS
198	198	100	100	100.0	59083	PASS
199	198	5	9	7.4	4351	PASS
275	198	10	60	24.8	14664	PASS
365	198	1	100	4.8	2854	PASS
441	198	0.01	100	11.5	6808	PASS
442	442	50	100	100.0	48776	PASS
443	442	15	24	20.7	10096	PASS