

Data File : BN004105.D

Acq On : 19 Dec 2018 10:15

Operator : JU/SJ

Sample : J6271-05DL 5X

Misc :

ALS Vial : 4 Sample Multiplier: 1




Quant Time: Dec 20 04:44:53 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Dec 20 04:42:11 2018

Response via : Initial Calibration

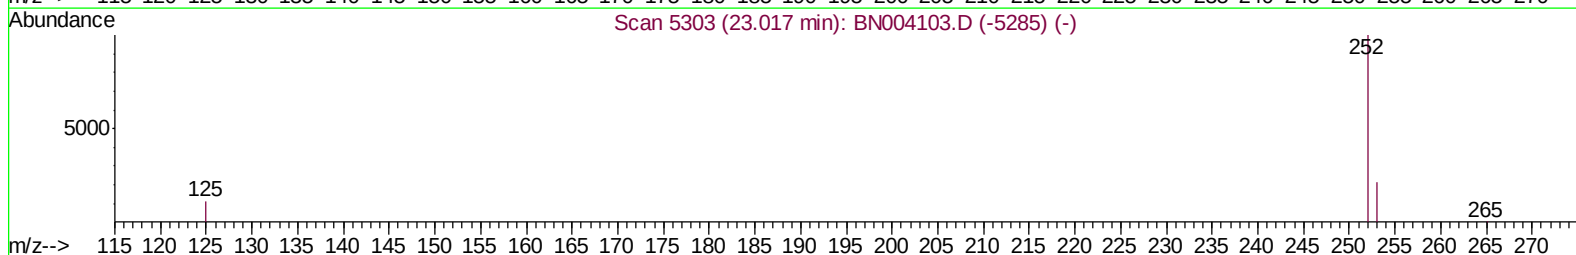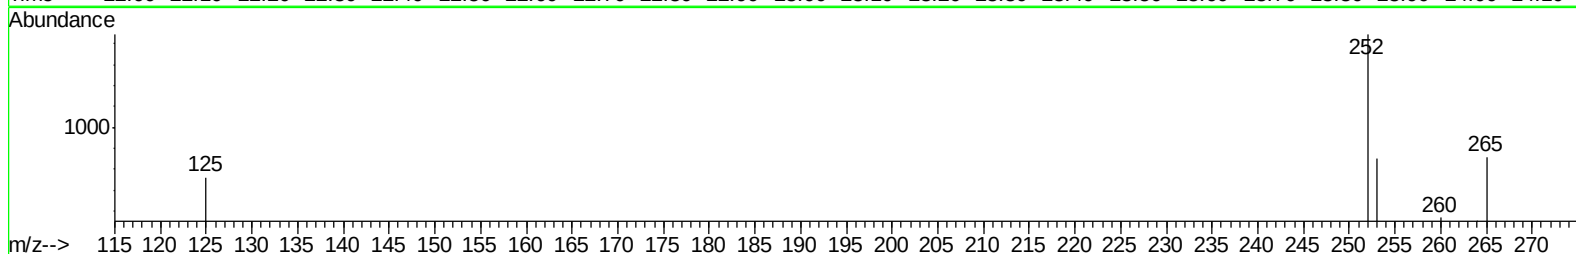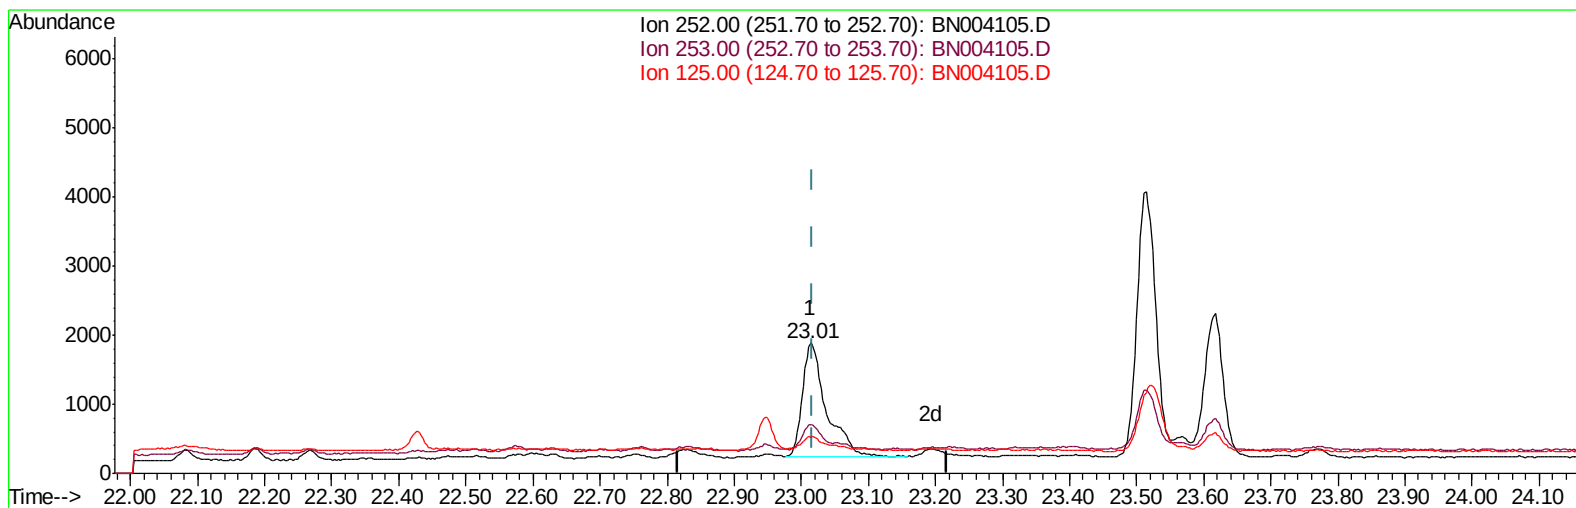

TIC: BN004105.D

(21) Benzo(b)fluoranthene

23.015min (-0.003) 0.09ng/ul

response 4043

Ion	Exp%	Act%
252.00	100	100
253.00	23.00	37.18
125.00	11.20	27.81#
0.00	0.00	0.00