
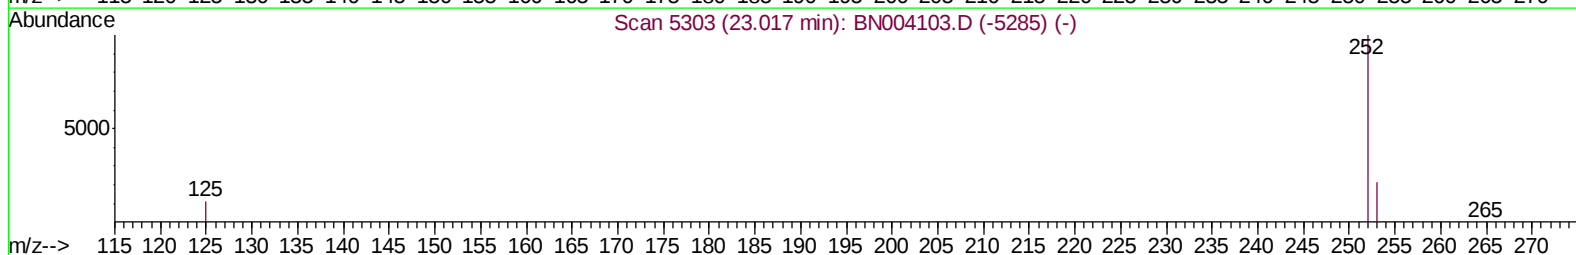
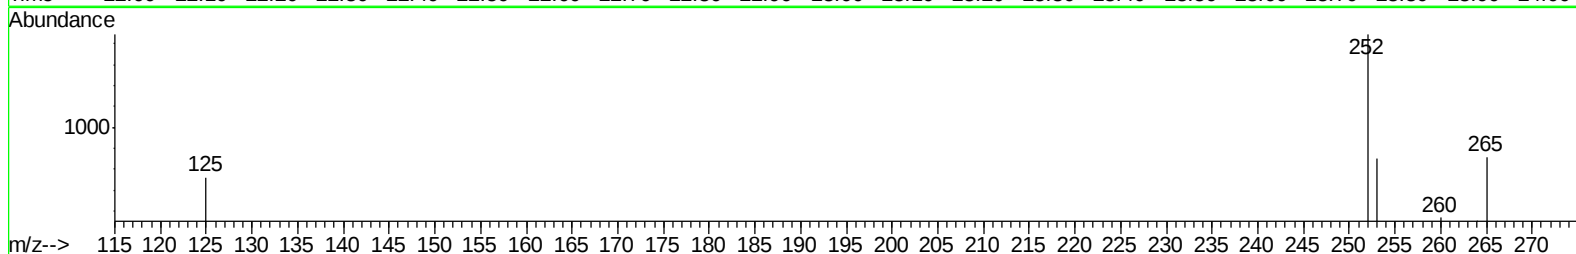


Data File : BN004105.D  
Acq On : 19 Dec 2018 10:15  
Operator : JU/SJ  
Sample : J6271-05DL 5X  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 20 04:44:53 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-SIM-BN111918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Dec 20 04:42:11 2018  
Response via : Initial Calibration

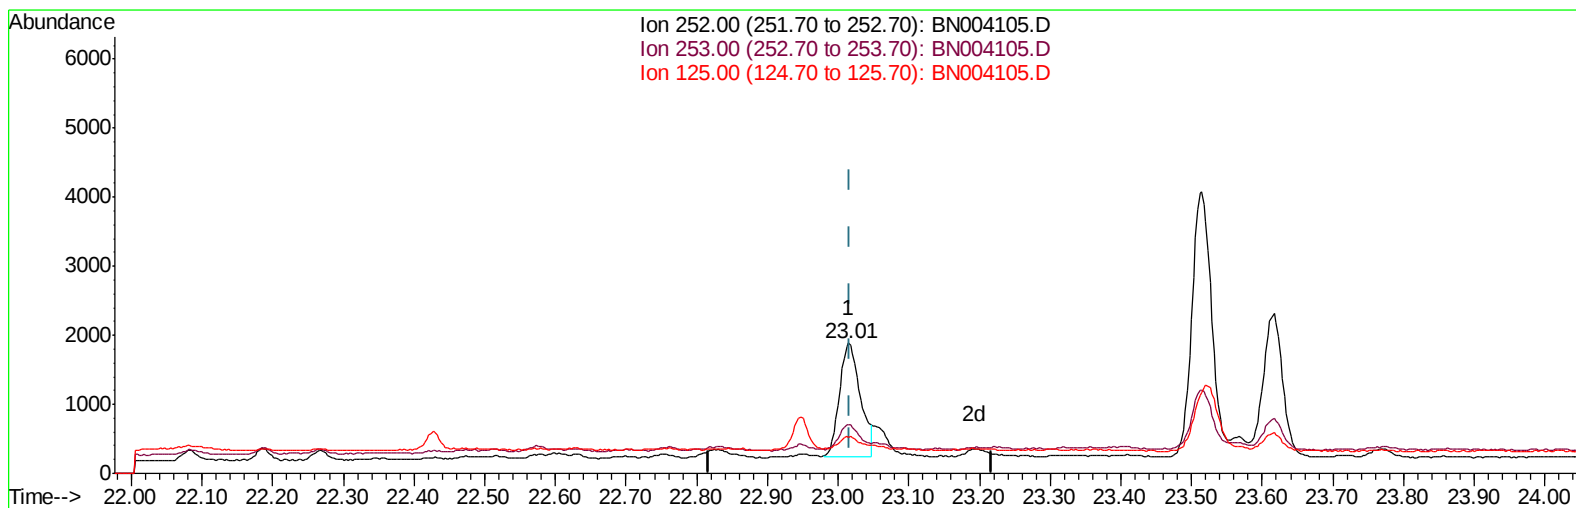

TIC: BN004105.D

(21) Benzo(b)fluoranthene

23.015min (-0.003) 0.07ng/ul m

response 3352

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 23.00 | 37.18  |
| 125.00 | 11.20 | 27.81# |
| 0.00   | 0.00  | 0.00   |