
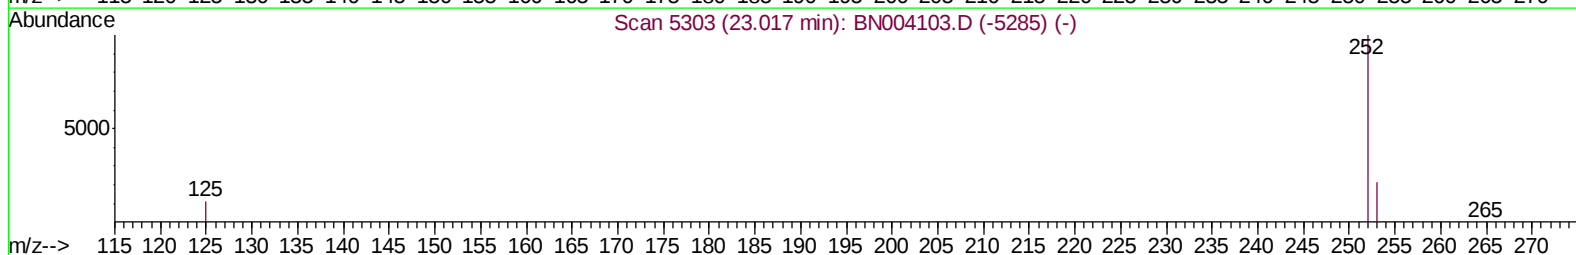
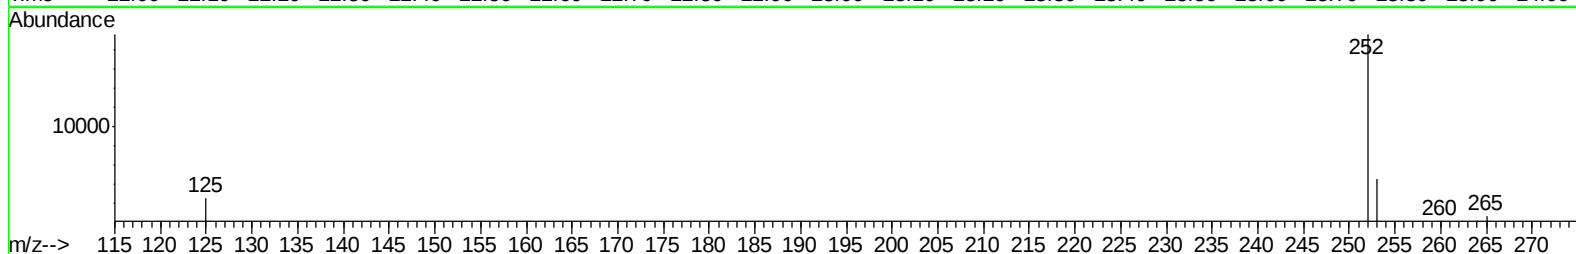


Data File : BN004107.D
Acq On : 19 Dec 2018 11:25
Operator : JU/SJ
Sample : J6271-13DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Dec 20 04:45:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 04:42:11 2018
Response via : Initial Calibration

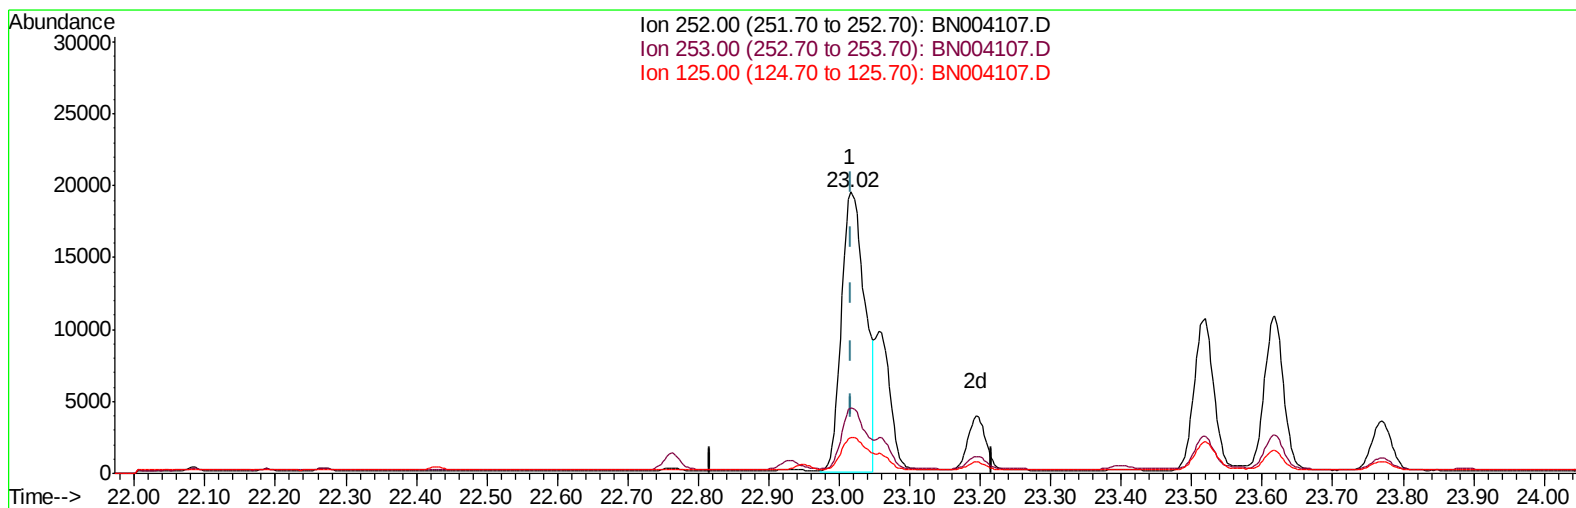

TIC: BN004107.D

(21) Benzo(b)fluoranthene

23.016min (-0.002) 0.96ng/ul m

response 45617

Ion	Exp%	Act%
252.00	100	100
253.00	23.00	23.28
125.00	11.20	12.77
0.00	0.00	0.00