
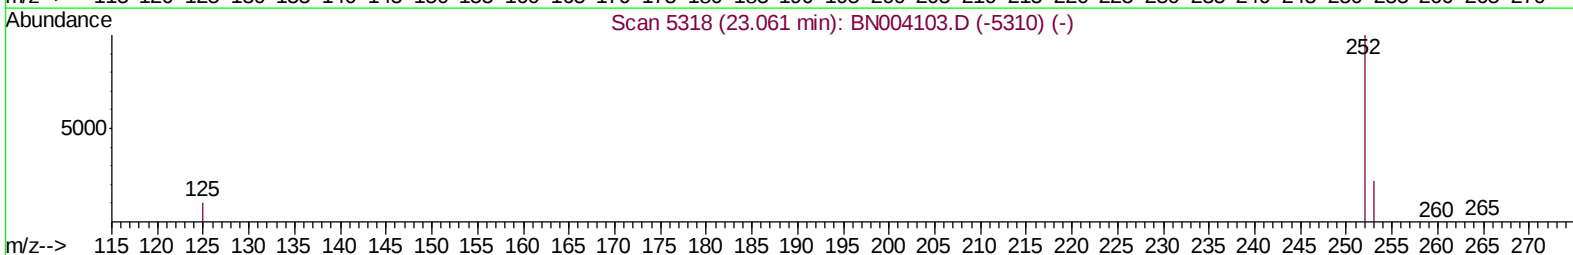
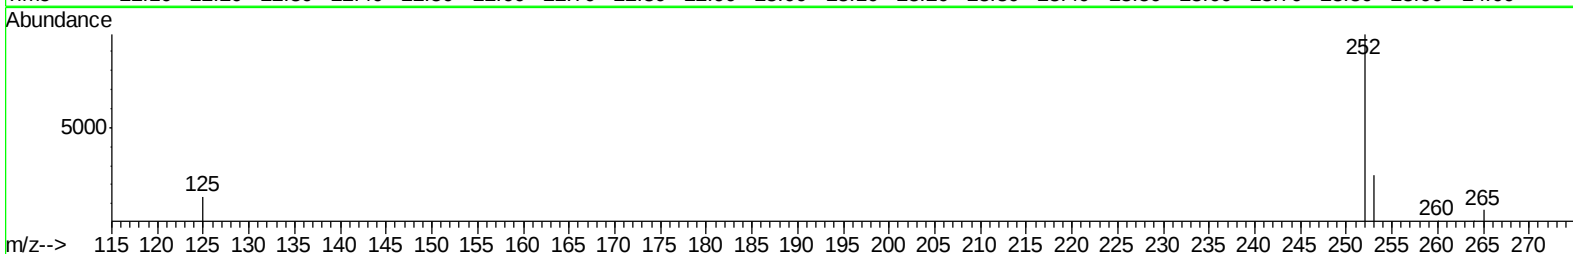


Data File : BN004107.D
Acq On : 19 Dec 2018 11:25
Operator : JU/SJ
Sample : J6271-13DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Dec 20 04:45:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 04:42:11 2018
Response via : Initial Calibration

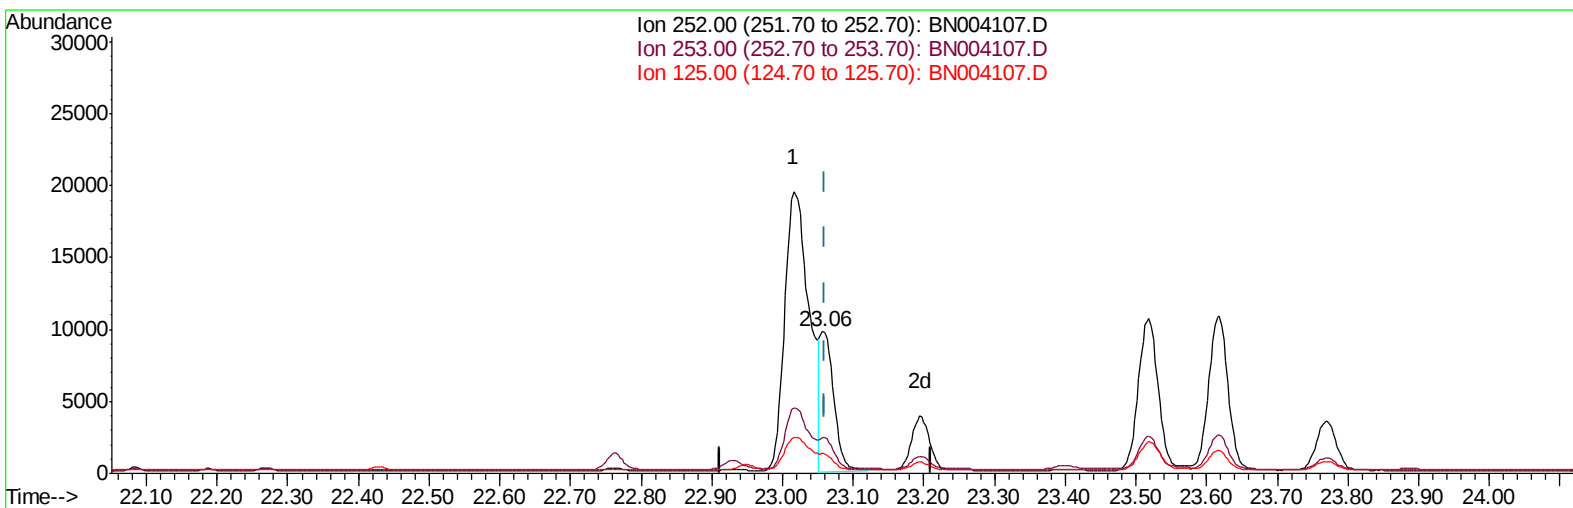

TIC: BN004107.D

(22) Benzo(k)fluoranthene

23.057min (-0.005) 0.28ng/ul m

response 13128

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	24.98
125.00	11.30	14.02#
0.00	0.00	0.00