
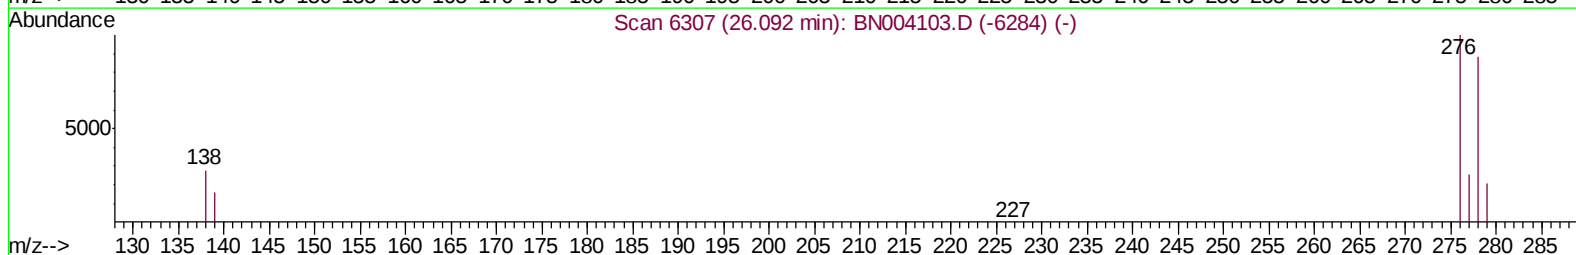
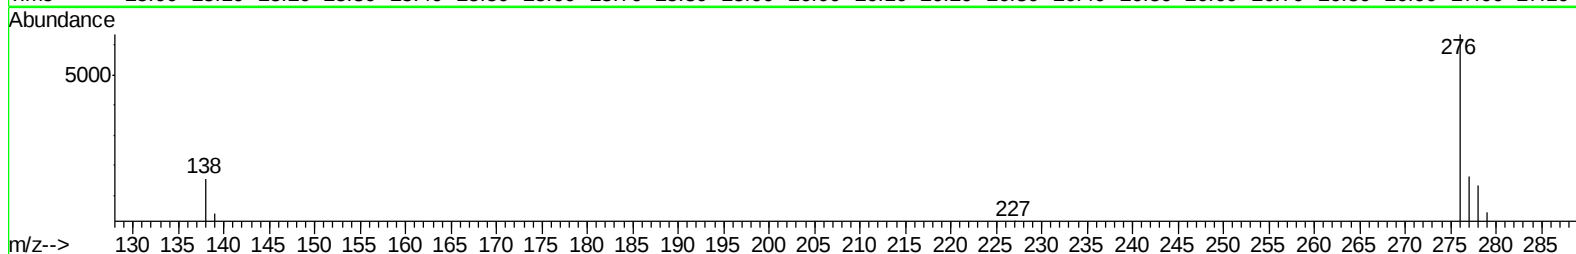


Data File : BN004107.D
Acq On : 19 Dec 2018 11:25
Operator : JU/SJ
Sample : J6271-13DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Dec 20 04:45:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 04:42:11 2018
Response via : Initial Calibration

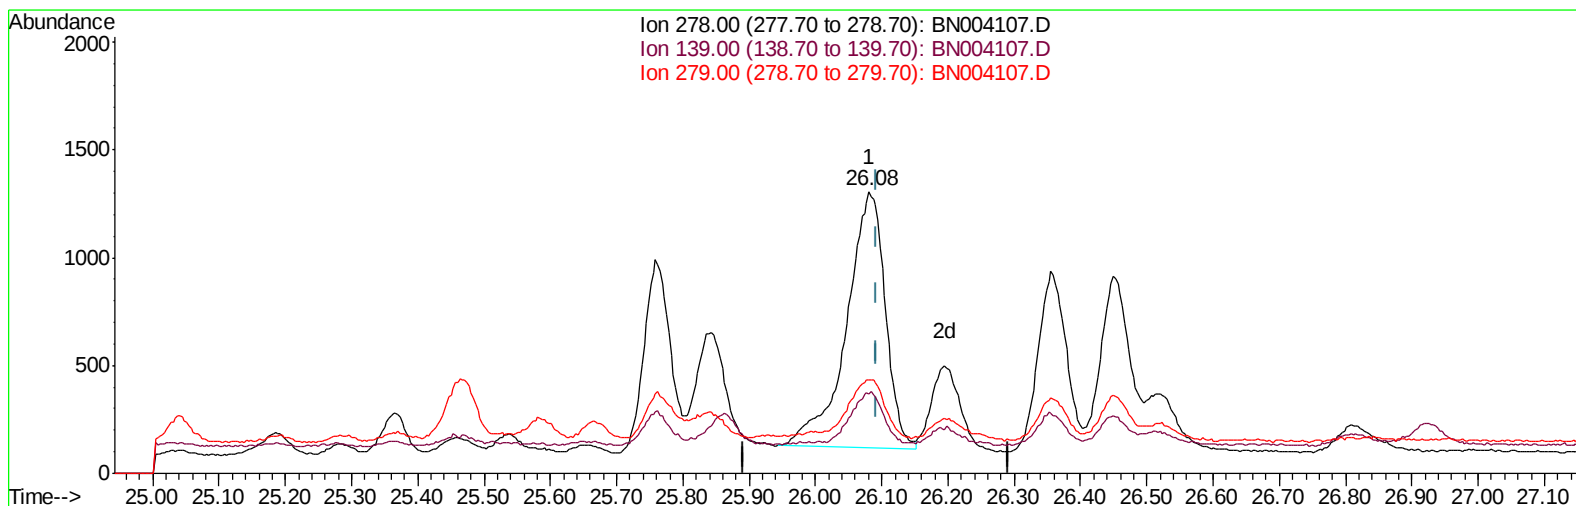

TIC: BN004107.D

(25) Dibenzo(a,h)anthracene

26.081min (-0.012) 0.13ng/ul

response 4842

Ion	Exp%	Act%
278.00	100	100
139.00	17.80	28.18#
279.00	24.70	33.15#
0.00	0.00	0.00