
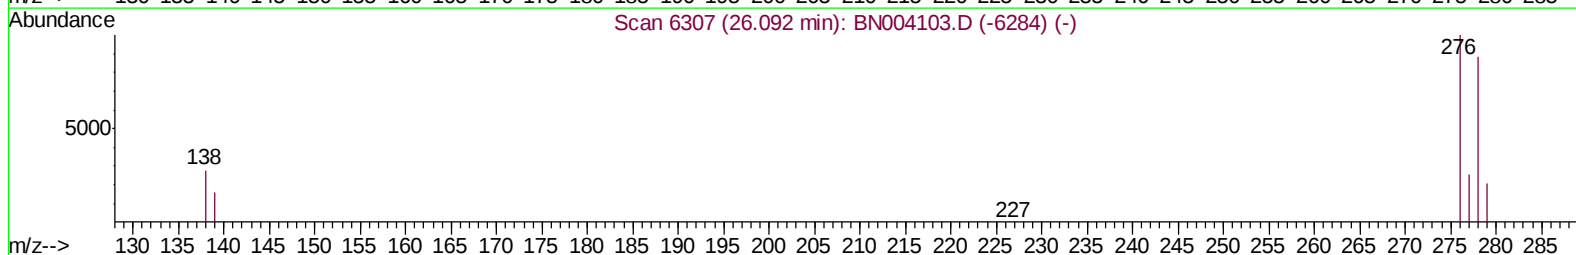
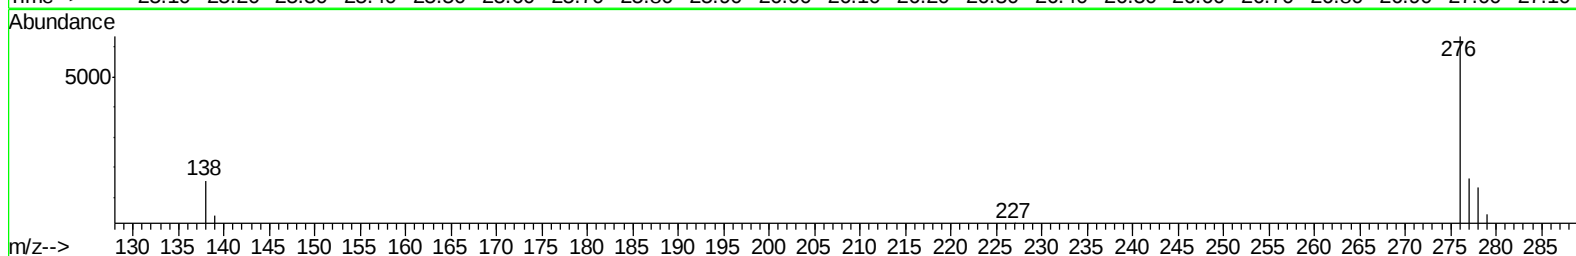


Data File : BN004107.D  
Acq On : 19 Dec 2018 11:25  
Operator : JU/SJ  
Sample : J6271-13DL 5X  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Dec 20 04:45:12 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-SIM-BN111918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Dec 20 04:42:11 2018  
Response via : Initial Calibration

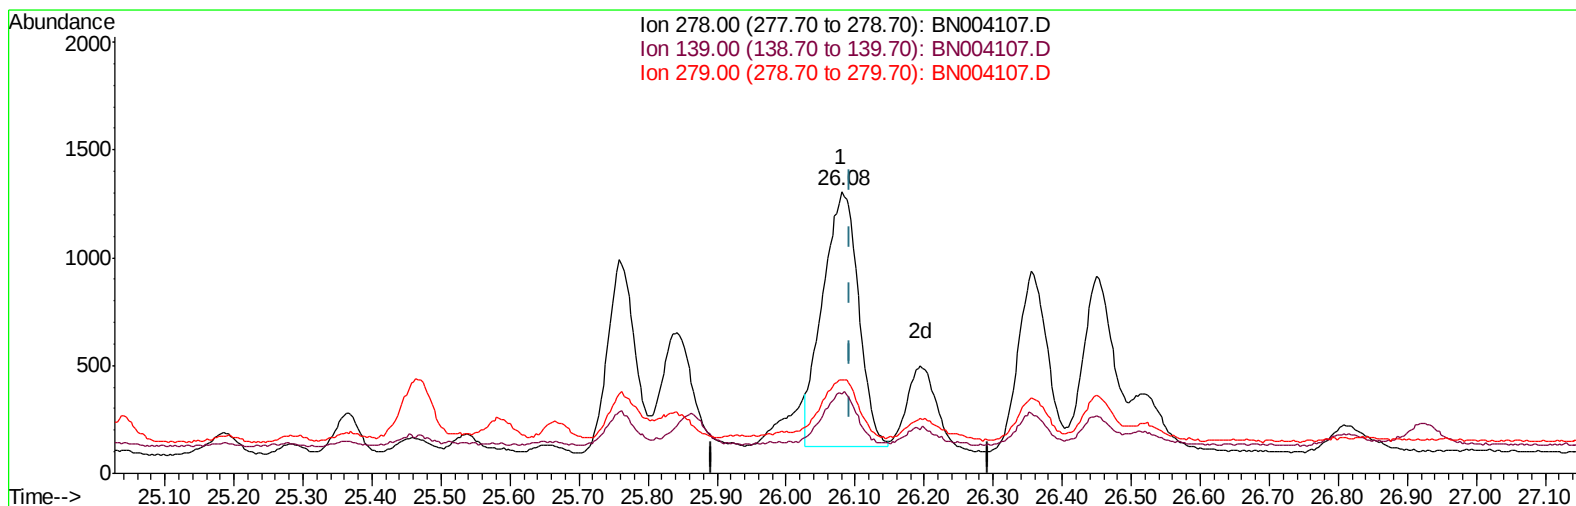

TIC: BN004107.D

(25) Dibenzo(a,h)anthracene

26.081min (-0.012) 0.11ng/ul m

response 4278

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 278.00 | 100   | 100    |
| 139.00 | 17.80 | 28.18# |
| 279.00 | 24.70 | 33.15# |
| 0.00   | 0.00  | 0.00   |