
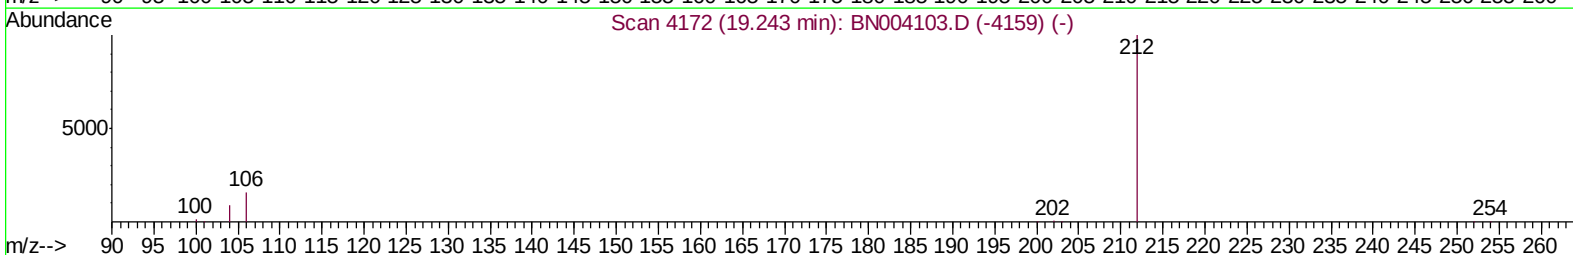
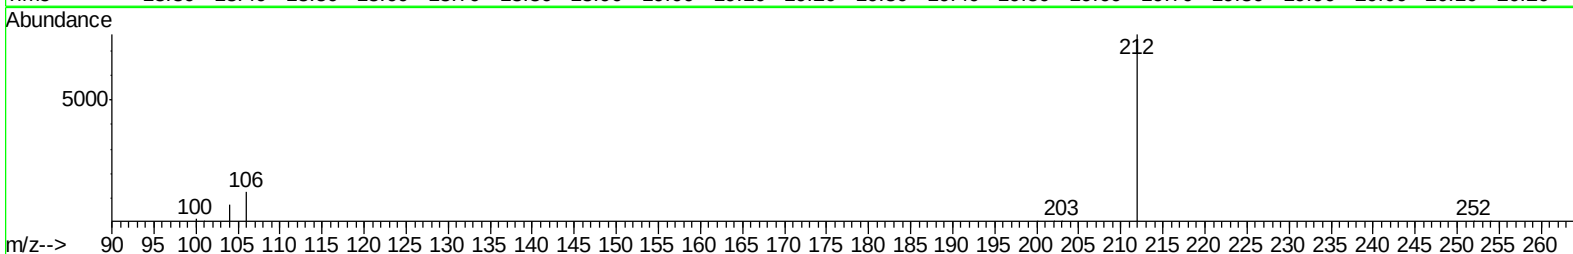


Data File : BN004108.D
Acq On : 19 Dec 2018 12:01
Operator : JU/SJ
Sample : PB115598BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Dec 20 04:56:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 04:42:11 2018
Response via : Initial Calibration

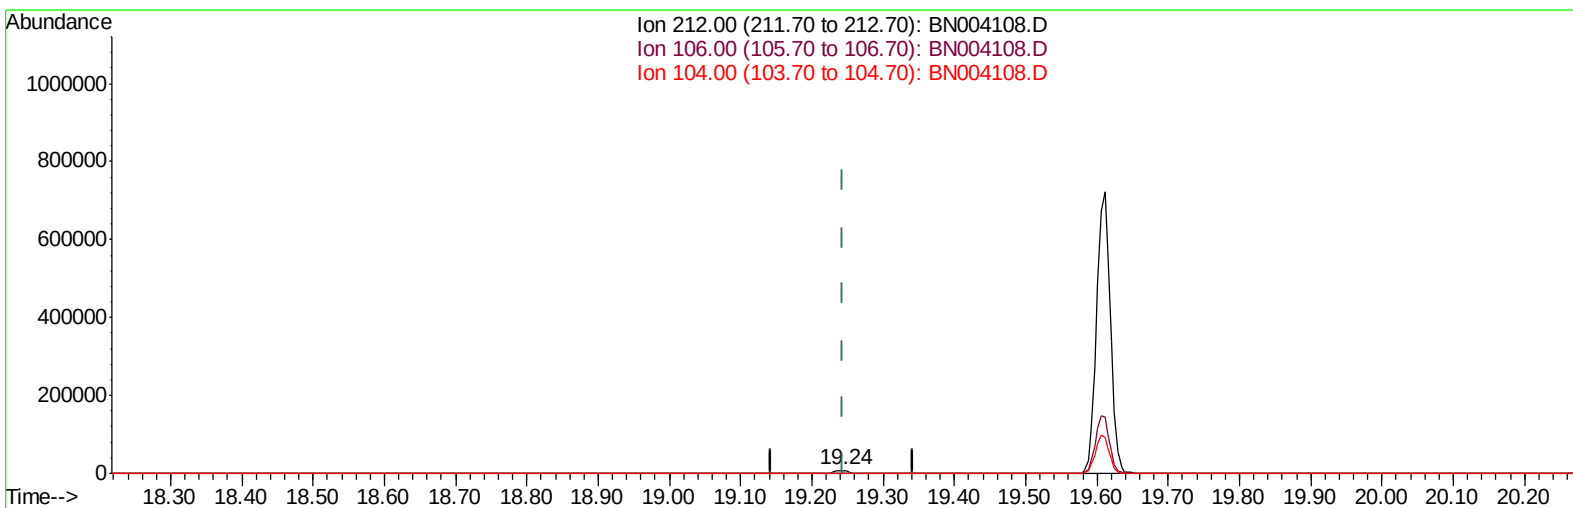

TIC: BN004108.D

(14) Fluoranthene-d10 (SURR)

19.244min (+0.000) 0.32ng/ul m

response 10350

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00