
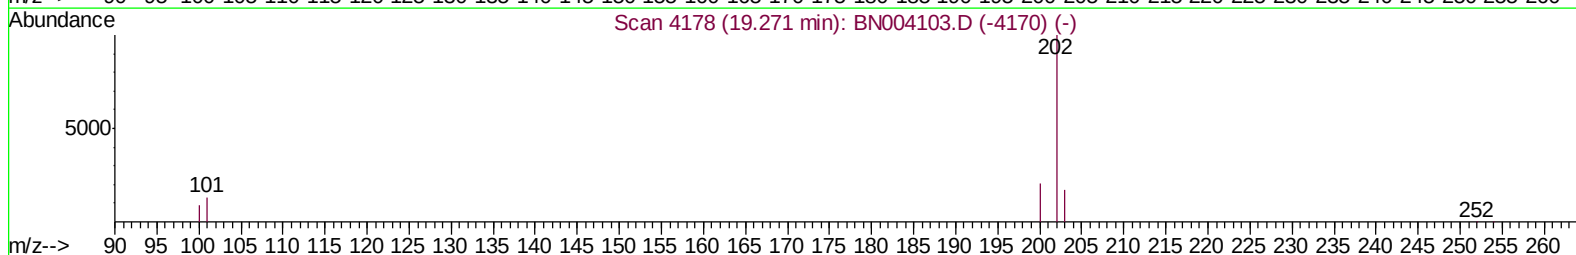
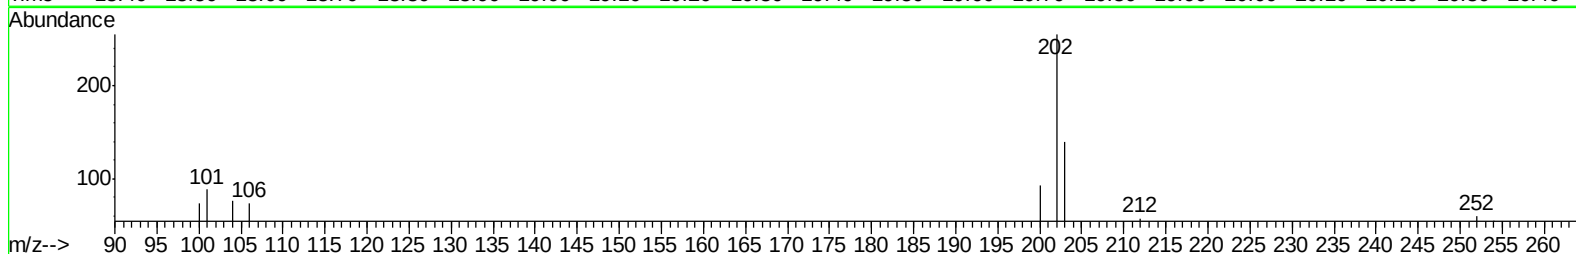


Data File : BN004109.D
Acq On : 19 Dec 2018 12:36
Operator : JU/SJ
Sample : J6297-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Dec 20 04:58:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 04:42:11 2018
Response via : Initial Calibration

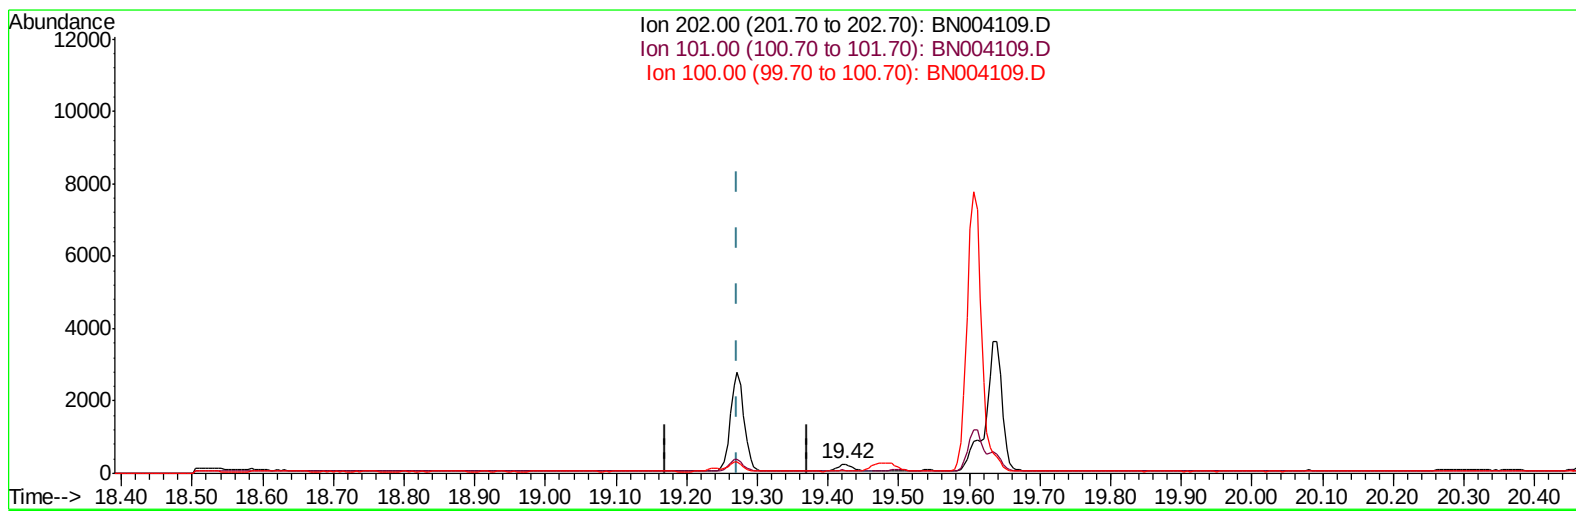

TIC: BN004109.D

(15) Fluoranthene (C)

19.425min (+0.153) 0.01ng/ul

response 269

Ion	Exp%	Act%
202.00	100	100
101.00	10.70	34.51#
100.00	8.10	28.63#
0.00	0.00	0.00