

Data File : BN004109.D

Acq On : 19 Dec 2018 12:36

Operator : JU/SJ

Sample : J6297-02

Misc :

ALS Vial : 8 Sample Multiplier: 1




Quant Time: Dec 20 05:01:26 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Dec 20 04:42:11 2018

Response via : Initial Calibration

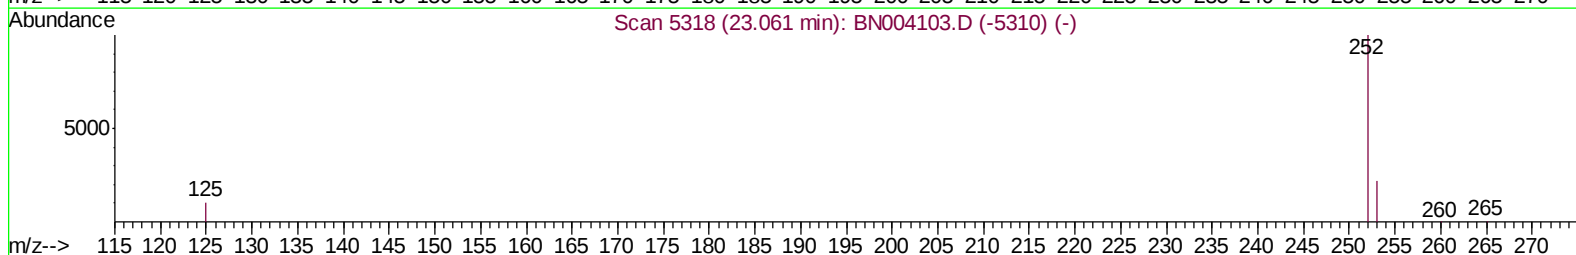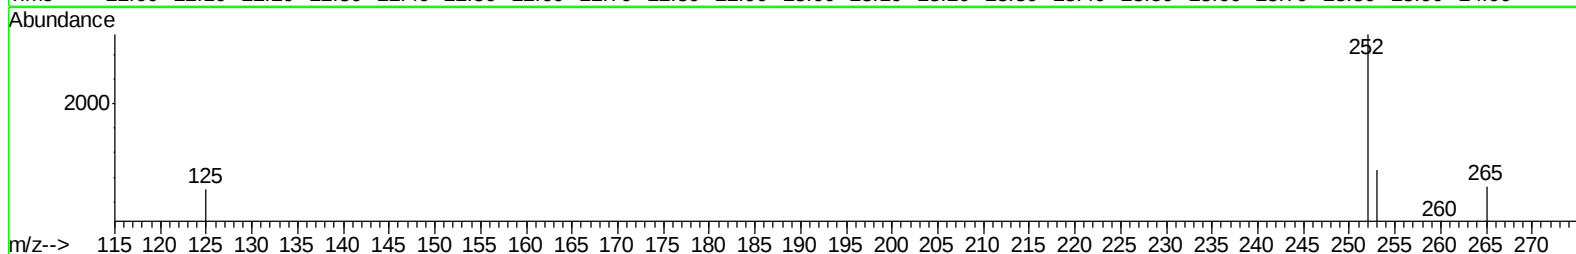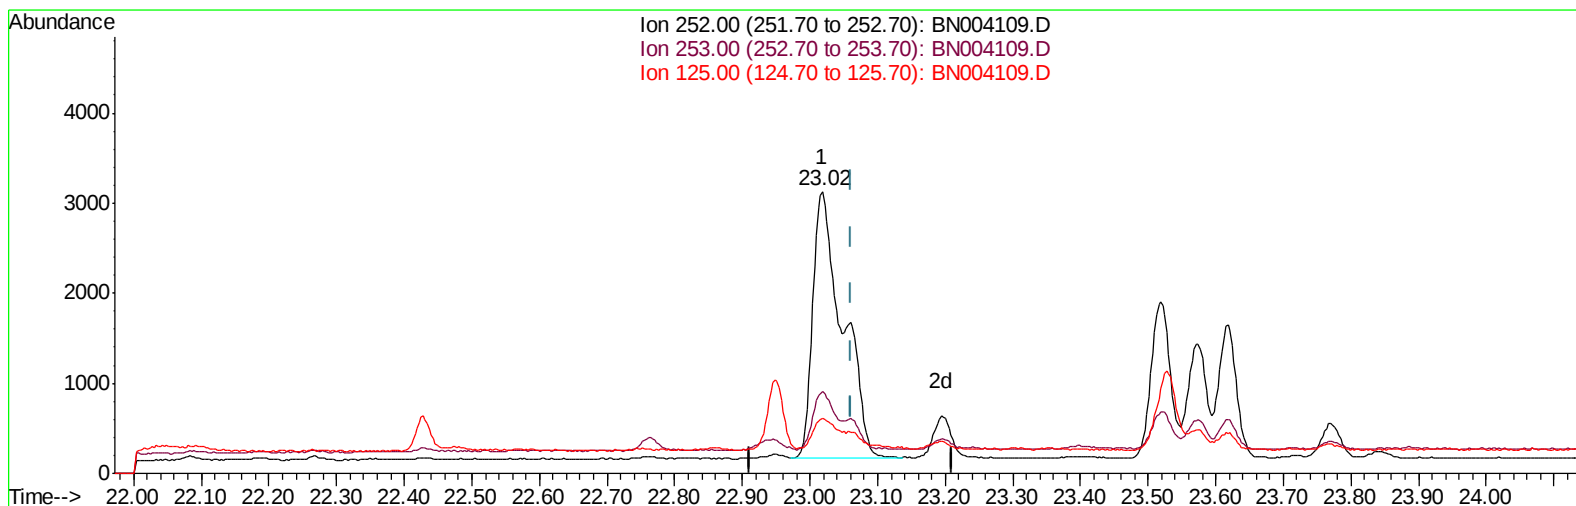

TIC: BN004109.D

(22) Benzo(k)fluoranthene

23.019min (-0.043) 0.21ng/ul

response 9075

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	29.27#
125.00	11.30	19.35#
0.00	0.00	0.00