

Data File : BN004109.D

Acq On : 19 Dec 2018 12:36

Operator : JU/SJ

Sample : J6297-02

Misc :

ALS Vial : 8 Sample Multiplier: 1




Quant Time: Dec 20 05:01:26 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Dec 20 04:42:11 2018

Response via : Initial Calibration

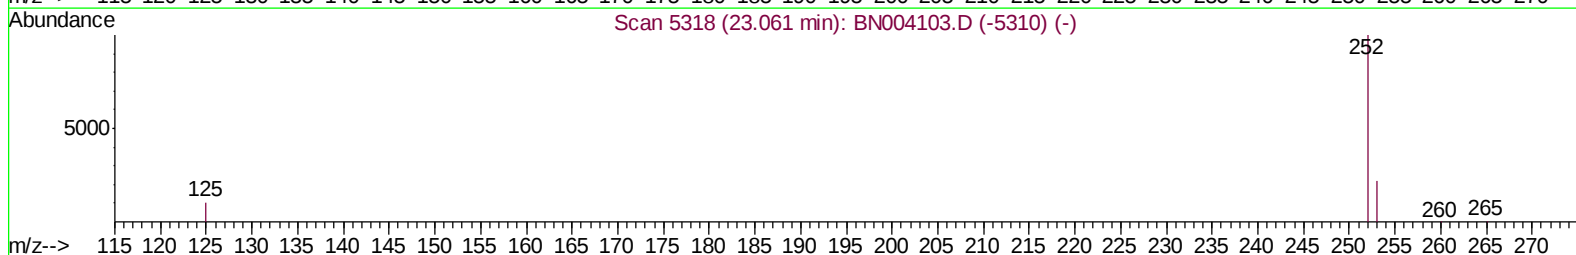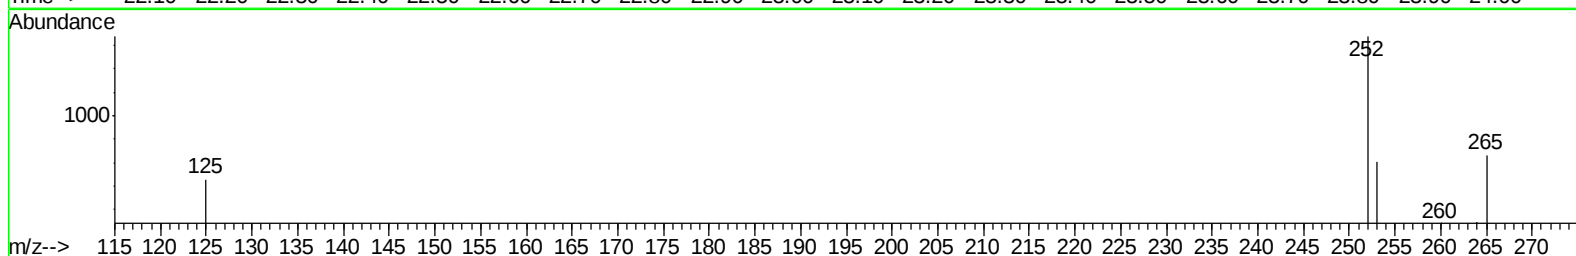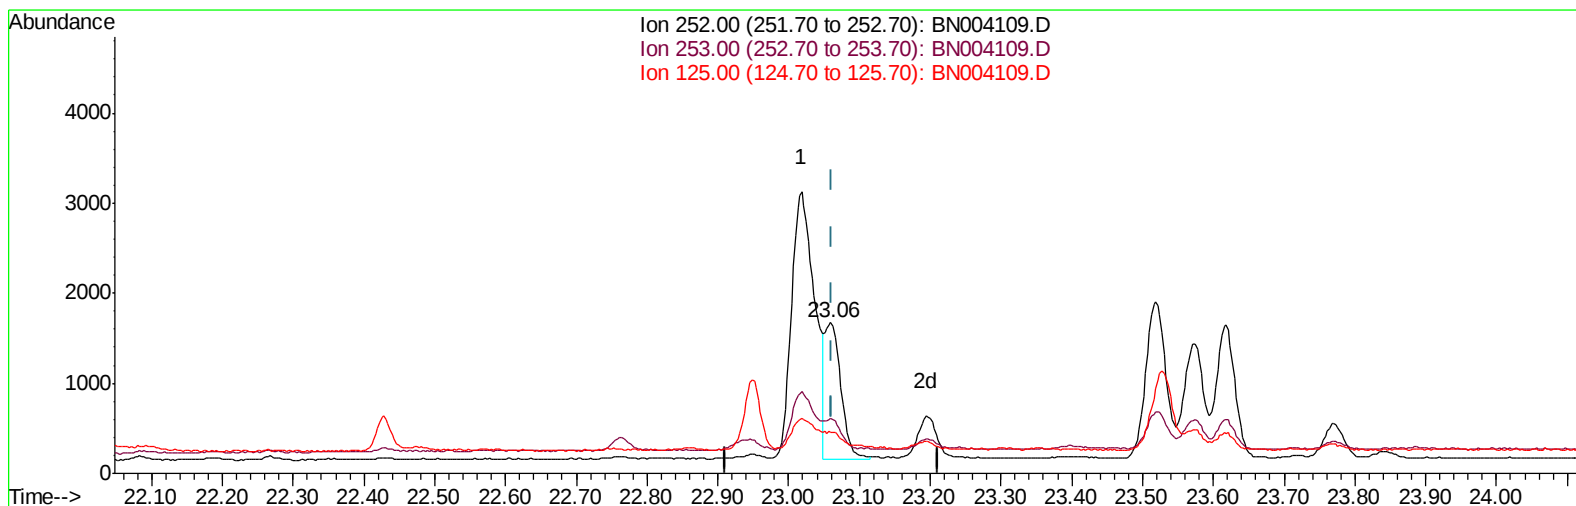

TIC: BN004109.D

(22) Benzo(k)fluoranthene

23.060min (-0.002) 0.06ng/ul m

response 2449

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	36.14#
125.00	11.30	27.18#
0.00	0.00	0.00