

Data File : BN004110.D

Acq On : 19 Dec 2018 13:11

Operator : JU/SJ

Sample : J6297-03

Misc :

ALS Vial : 9 Sample Multiplier: 1




Quant Time: Dec 20 05:33:01 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Dec 20 04:42:11 2018

Response via : Initial Calibration

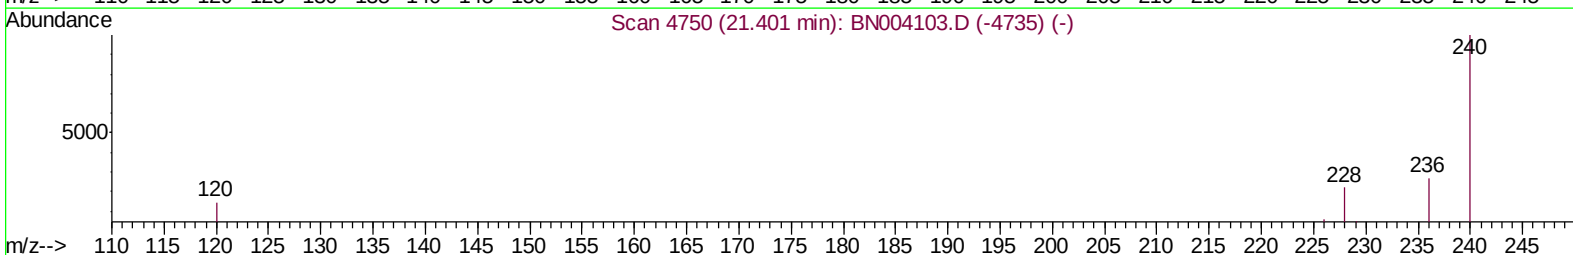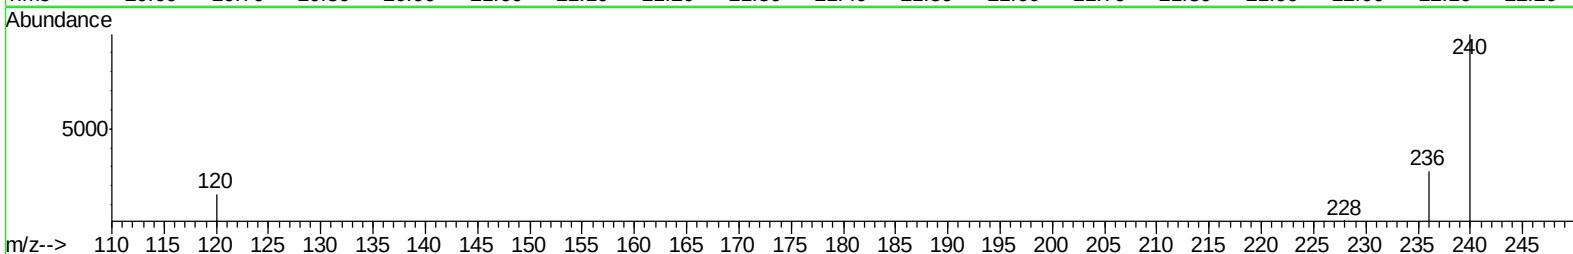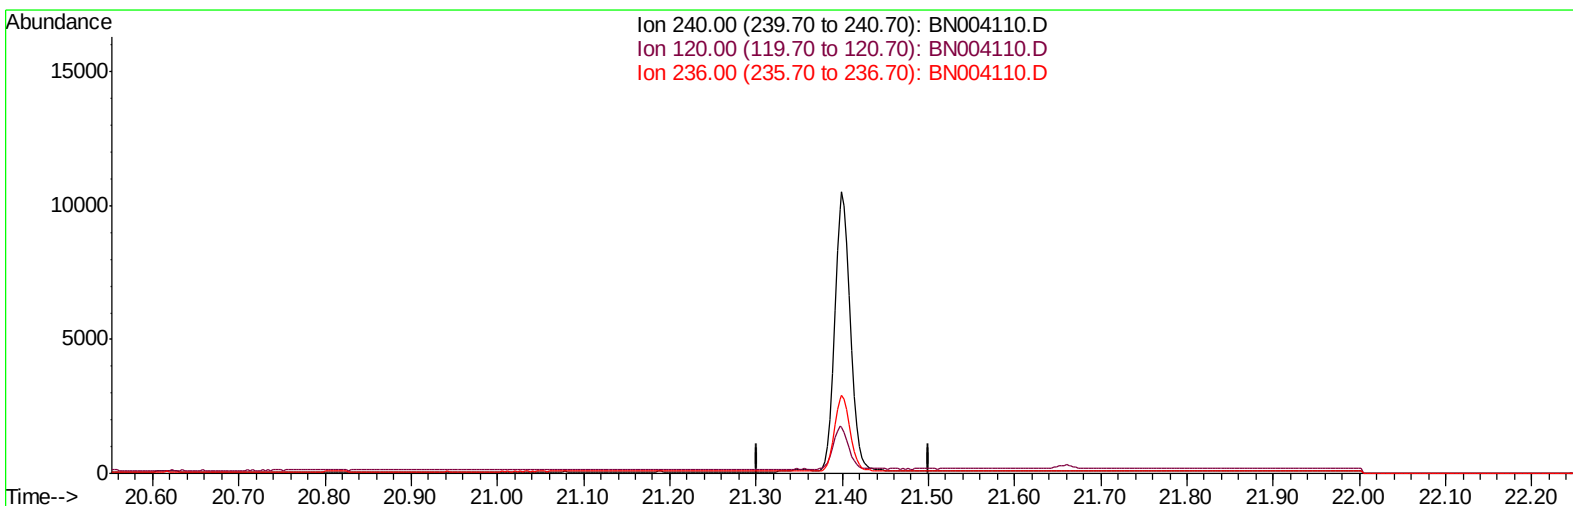

TIC: BN004110.D

(16) Chrysene-d12 (I)

21.401min (-21.401) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00