
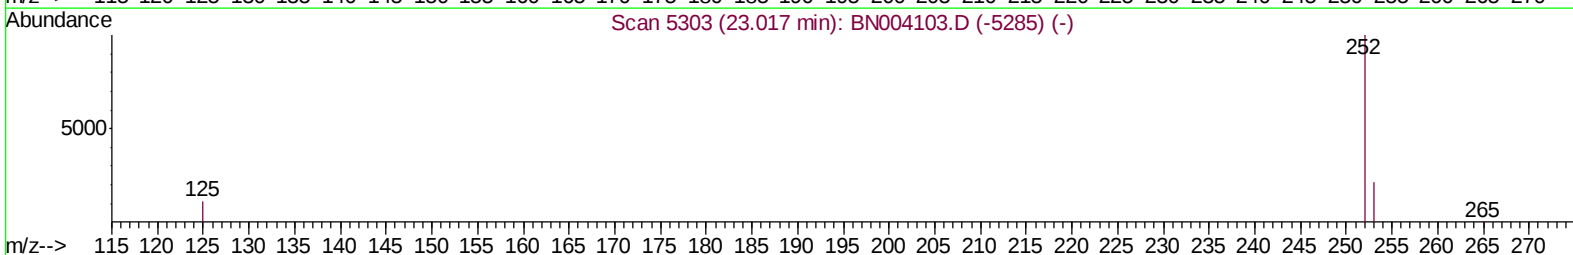
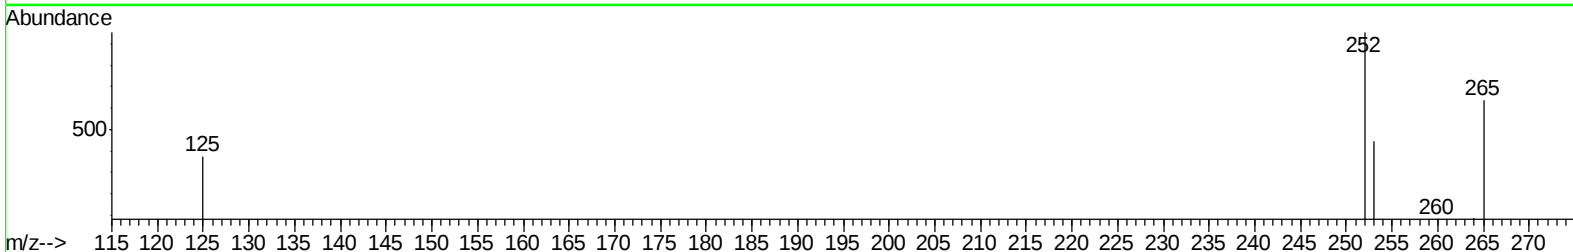


Data File : BN004112.D
Acq On : 19 Dec 2018 14:21
Operator : JU/SJ
Sample : J6297-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Dec 20 05:39:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN11918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 04:42:11 2018
Response via : Initial Calibration

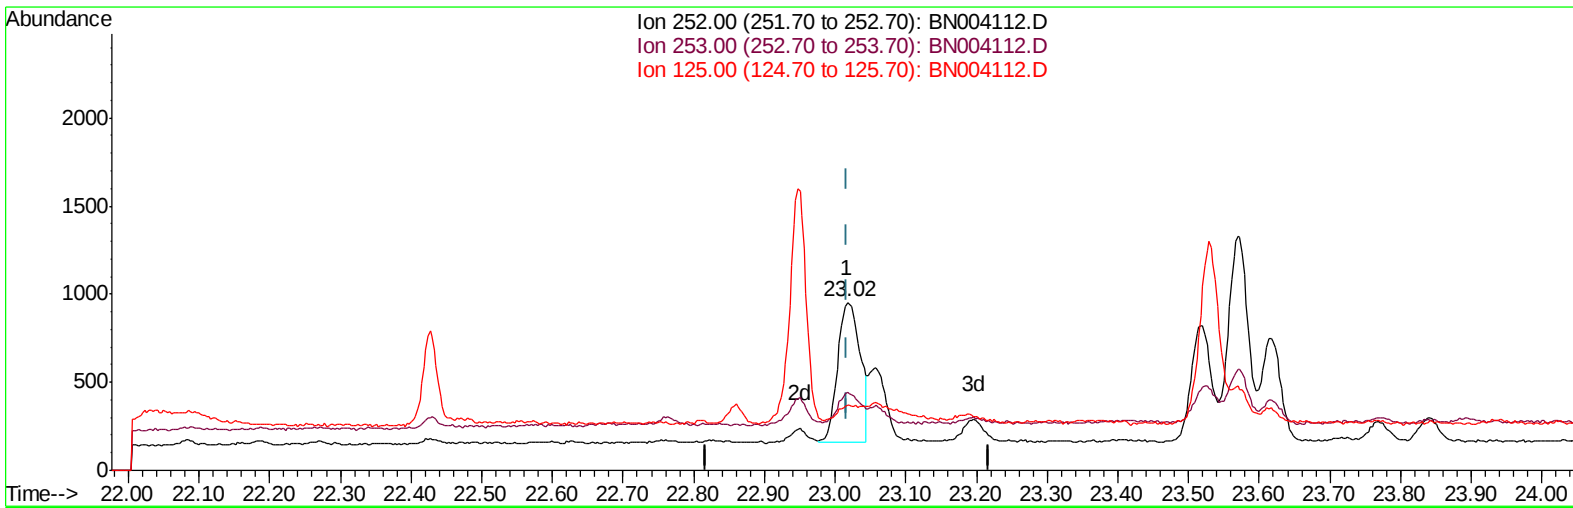

TIC: BN004112.D

(21) Benzo(b)fluoranthene

23.017min (-0.000) 0.04ng/ul m

response 1771

Ion	Exp%	Act%
252.00	100	100
253.00	23.00	46.80#
125.00	11.20	38.93#
0.00	0.00	0.00