
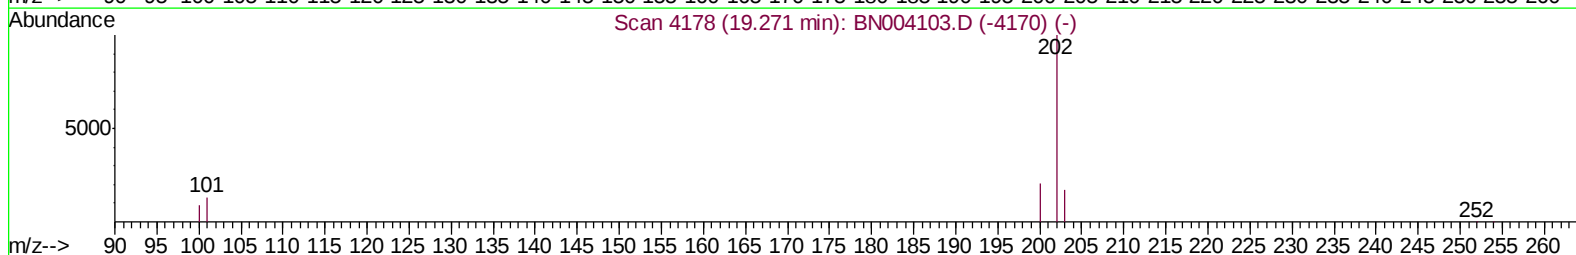
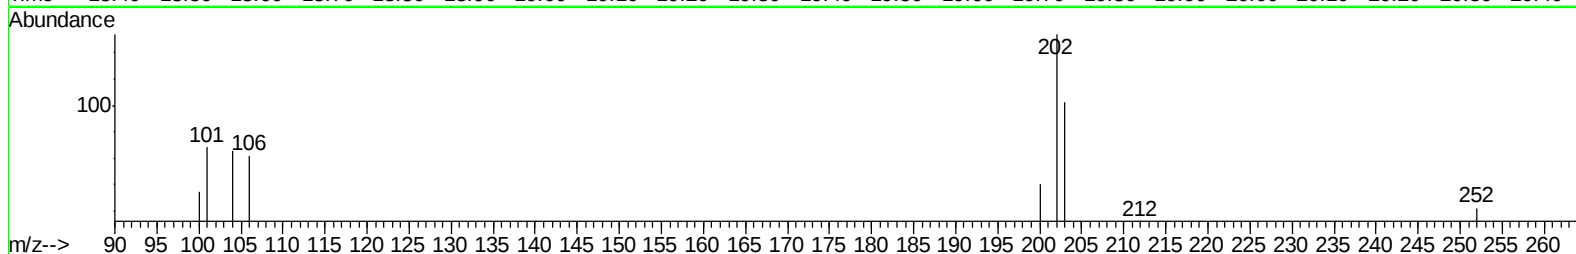


Data File : BN004114.D
Acq On : 19 Dec 2018 15:32
Operator : JU/SJ
Sample : J6297-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Dec 20 05:46:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 04:42:11 2018
Response via : Initial Calibration

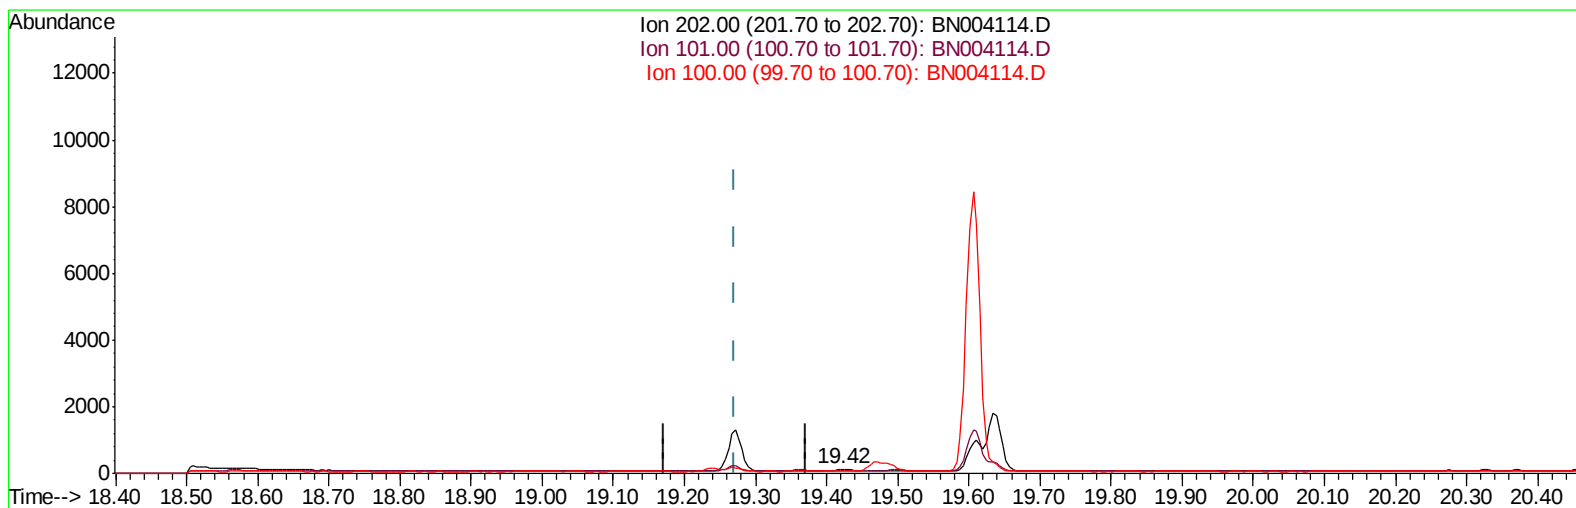

TIC: BN004114.D

(15) Fluoranthene (C)

19.420min (+0.149) 0.00ng/ul

response 81

Ion	Exp%	Act%
202.00	100	100
101.00	10.70	66.14#
100.00	8.10	52.76#
0.00	0.00	0.00