
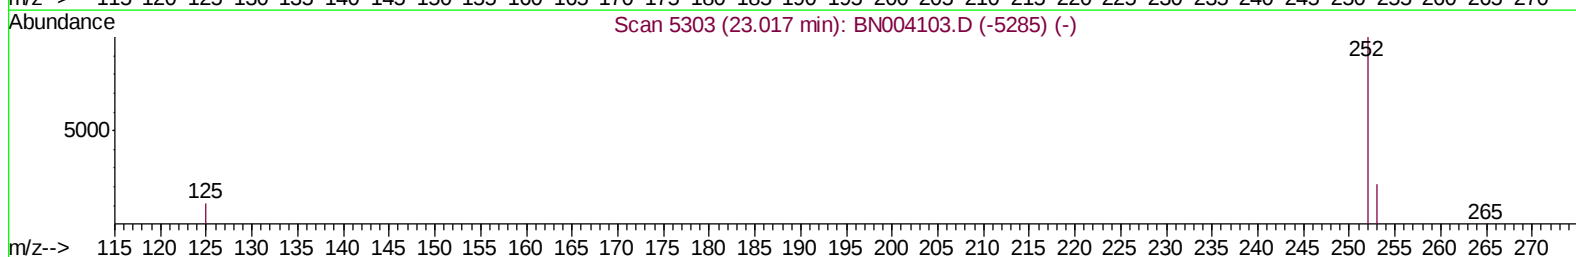
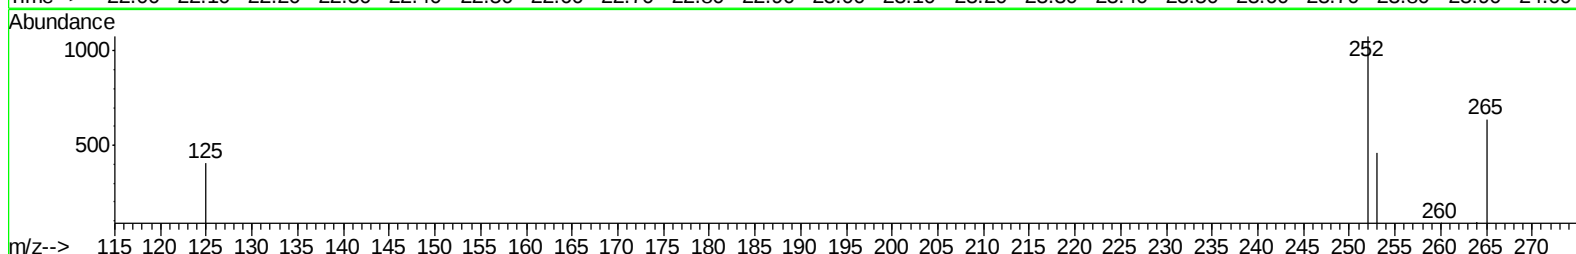


Data File : BN004114.D
Acq On : 19 Dec 2018 15:32
Operator : JU/SJ
Sample : J6297-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Dec 20 05:48:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 04:42:11 2018
Response via : Initial Calibration

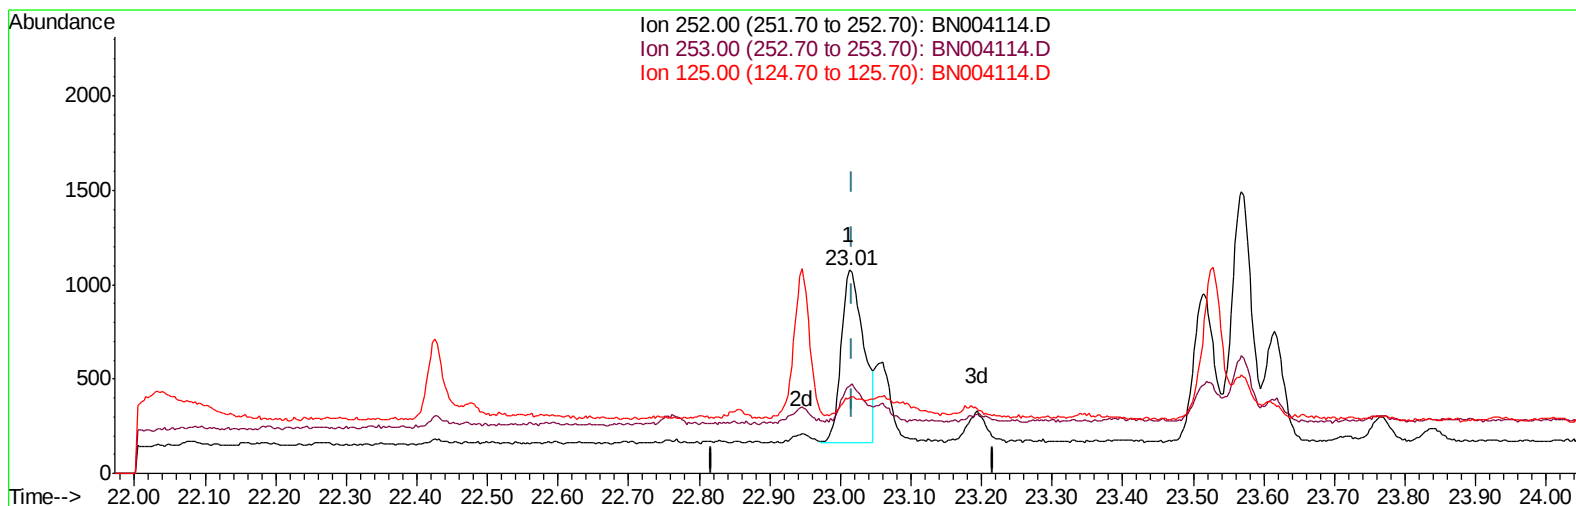

TIC: BN004114.D

(21) Benzo(b)fluoranthene

23.013min (-0.005) 0.05ng/ul m

response 2002

Ion	Exp%	Act%
252.00	100	100
253.00	23.00	42.80
125.00	11.20	37.42#
0.00	0.00	0.00