
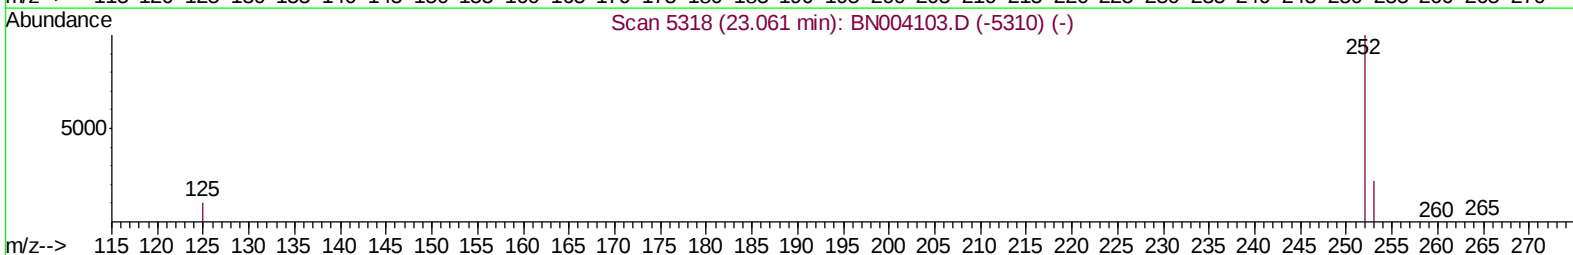
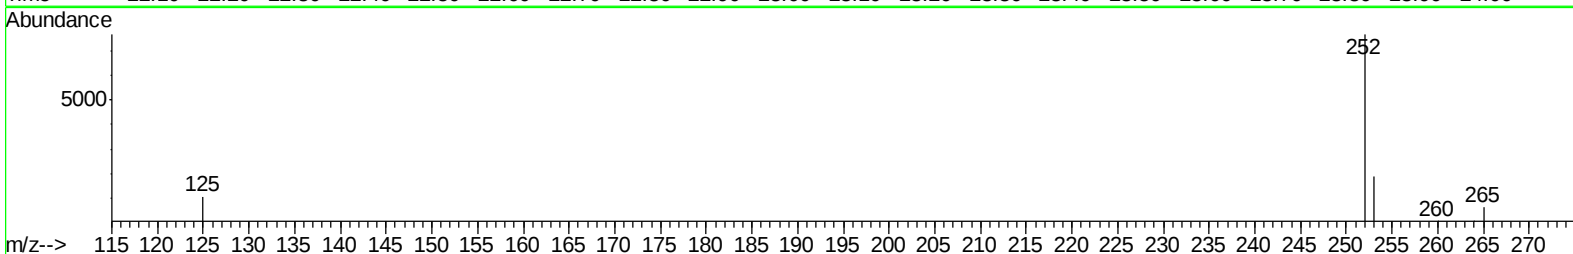


Data File : BN004115.D
Acq On : 19 Dec 2018 16:07
Operator : JU/SJ
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Dec 20 04:46:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 04:42:11 2018
Response via : Initial Calibration

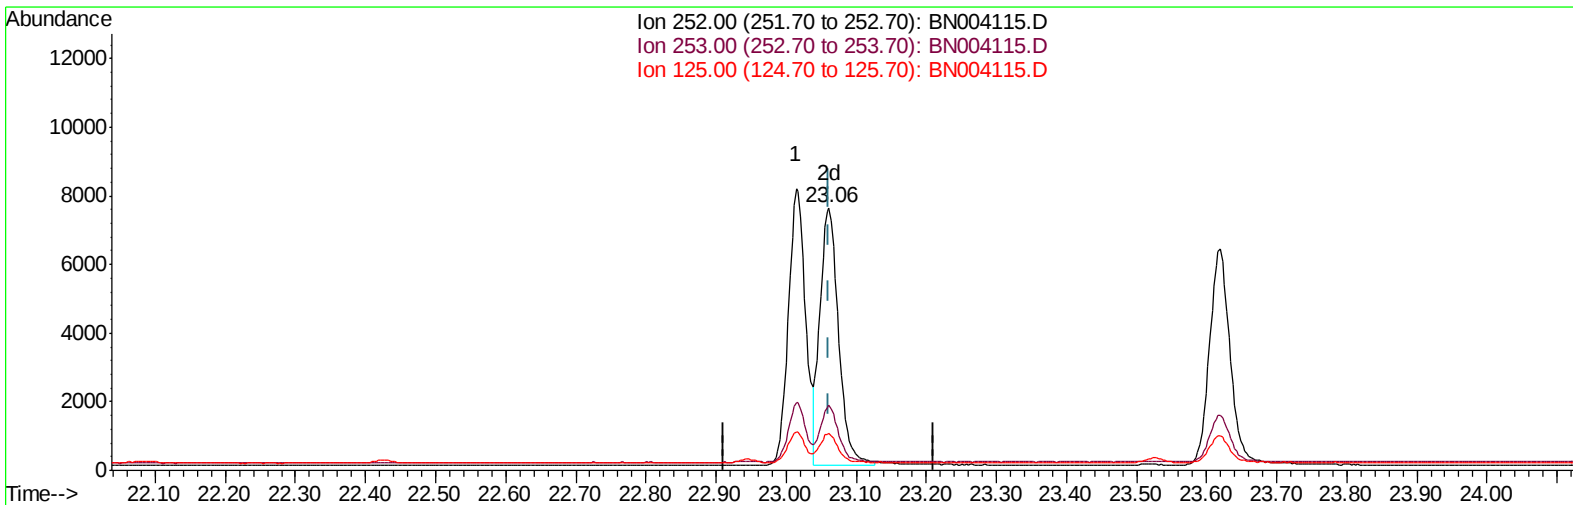

TIC: BN004115.D

(22) Benzo(k)fluoranthene

23.061min (-0.000) 0.38ng/ul m

response 13985

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	24.63
125.00	11.30	13.98#
0.00	0.00	0.00