
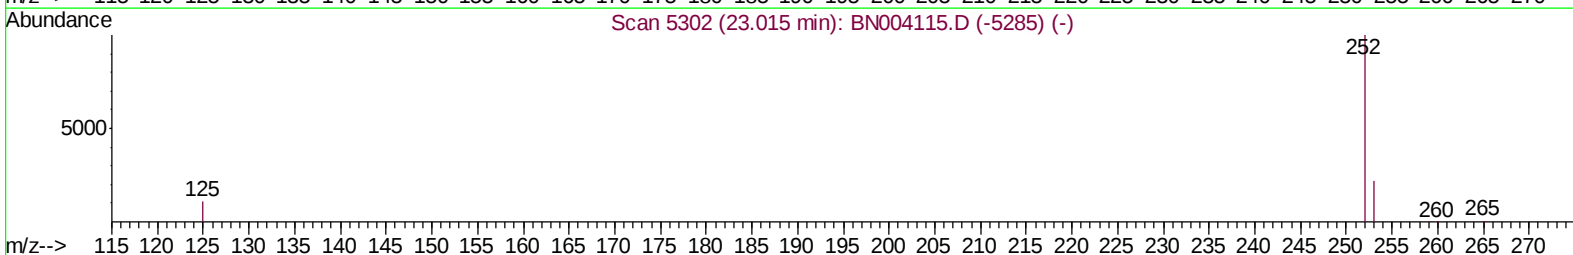
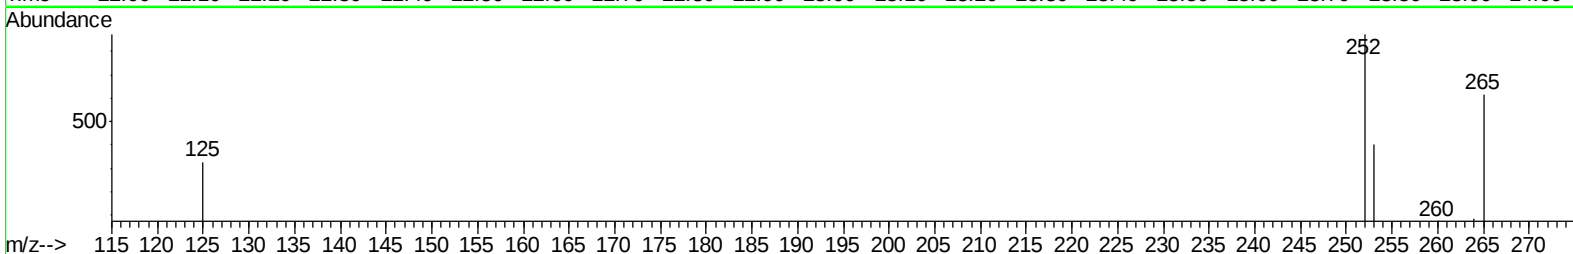


Data File : BN004116.D
Acq On : 19 Dec 2018 16:42
Operator : JU/SJ
Sample : J6297-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 20 05:59:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 05:49:27 2018
Response via : Initial Calibration

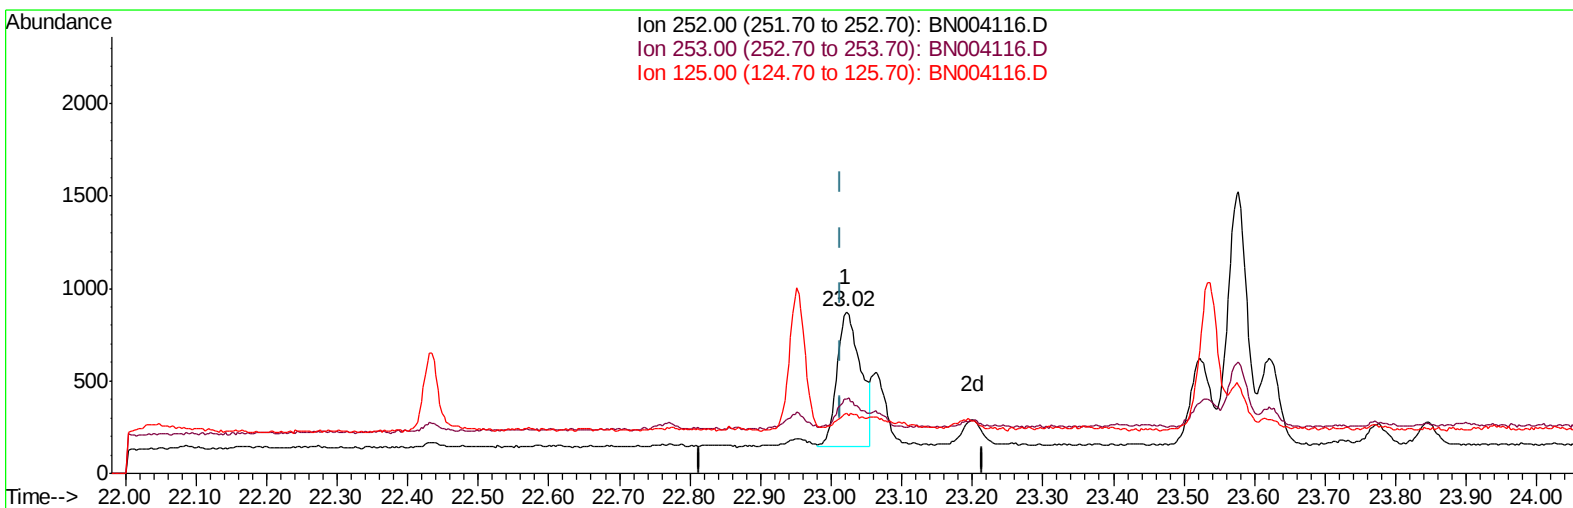

TIC: BN004116.D

(21) Benzo(b)fluoranthene

23.022min (+0.007) 0.04ng/ul m

response 1670

Ion	Exp%	Act%
252.00	100	100
253.00	23.00	46.39#
125.00	11.20	37.57#
0.00	0.00	0.00