
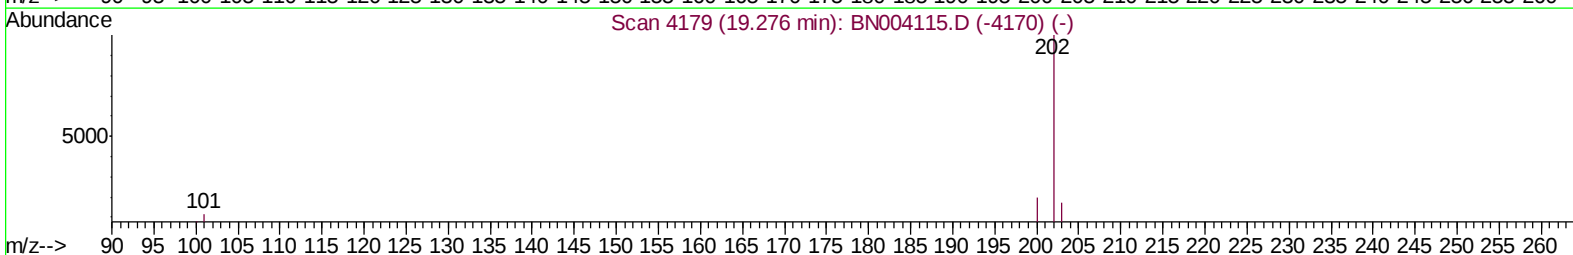
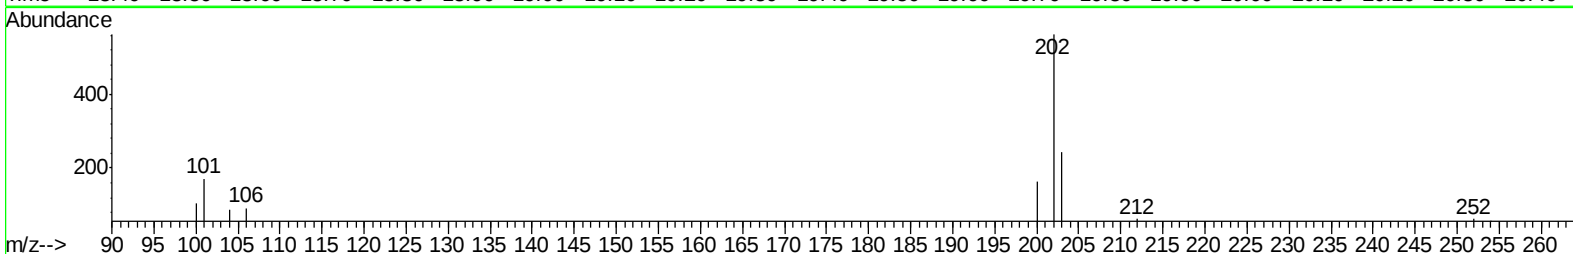


Data File : BN004118.D  
Acq On : 19 Dec 2018 17:53  
Operator : JU/SJ  
Sample : J6297-01  
Misc :  
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Dec 20 06:04:36 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-SIM-BN111918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Dec 20 05:49:27 2018  
Response via : Initial Calibration

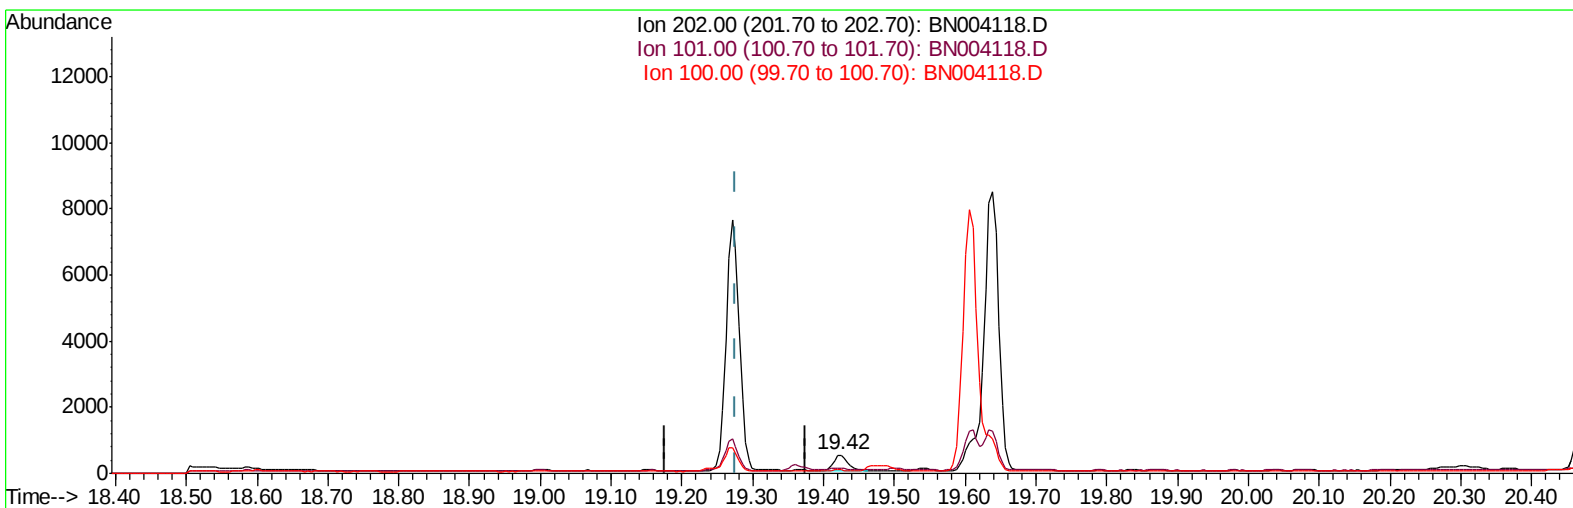

TIC: BN004118.D

(15) Fluoranthene (C)

19.425min (+0.149) 0.02ng/ul

response 654

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 202.00 | 100   | 100   |
| 101.00 | 10.70 | 30.43 |
| 100.00 | 8.10  | 18.86 |
| 0.00   | 0.00  | 0.00  |