
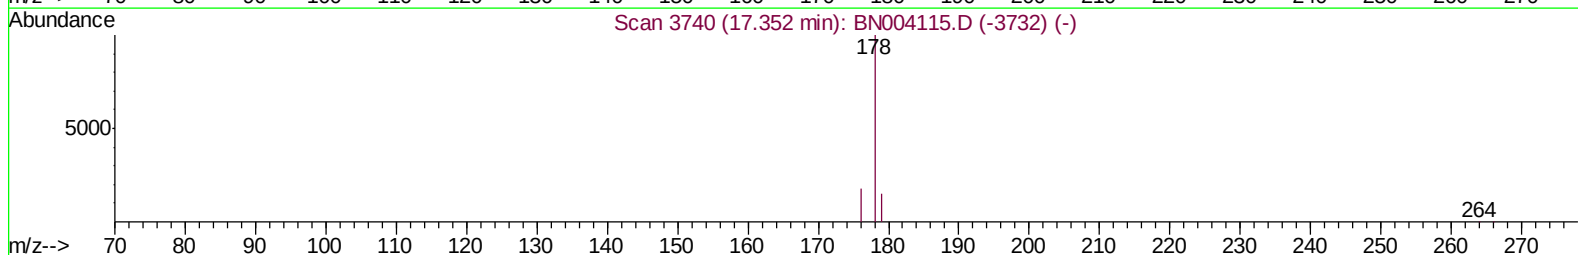
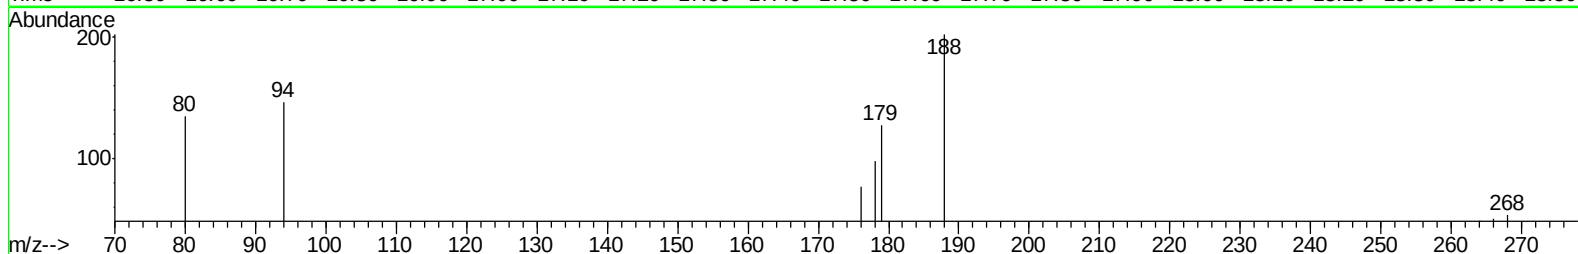


Data File : BN004121.D
Acq On : 19 Dec 2018 19:39
Operator : JU/SJ
Sample : J6297-11
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Dec 20 06:14:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 05:49:27 2018
Response via : Initial Calibration

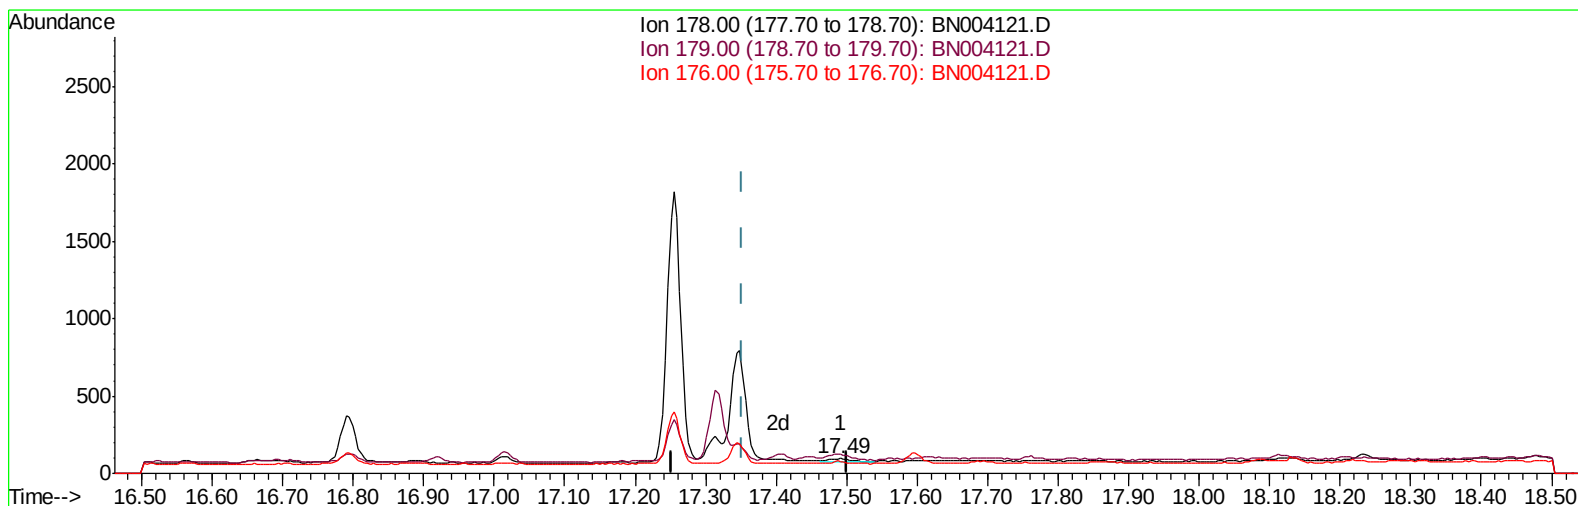

TIC: BN004121.D

(13) Anthracene

17.492min (+0.140) 0.00ng/ul

response 45

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	129.59#
176.00	18.50	77.55#
0.00	0.00	0.00