
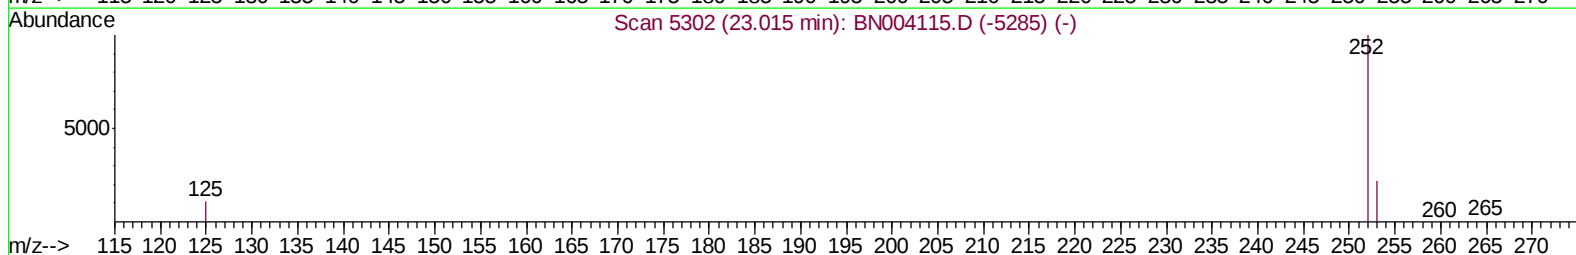
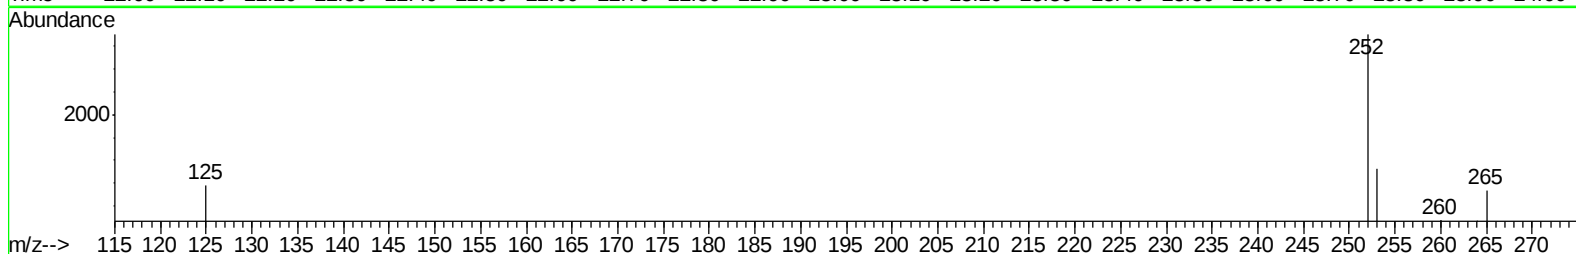


Data File : BN004121.D  
Acq On : 19 Dec 2018 19:39  
Operator : JU/SJ  
Sample : J6297-11  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Dec 20 06:17:18 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-SIM-BN11918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Dec 20 05:49:27 2018  
Response via : Initial Calibration

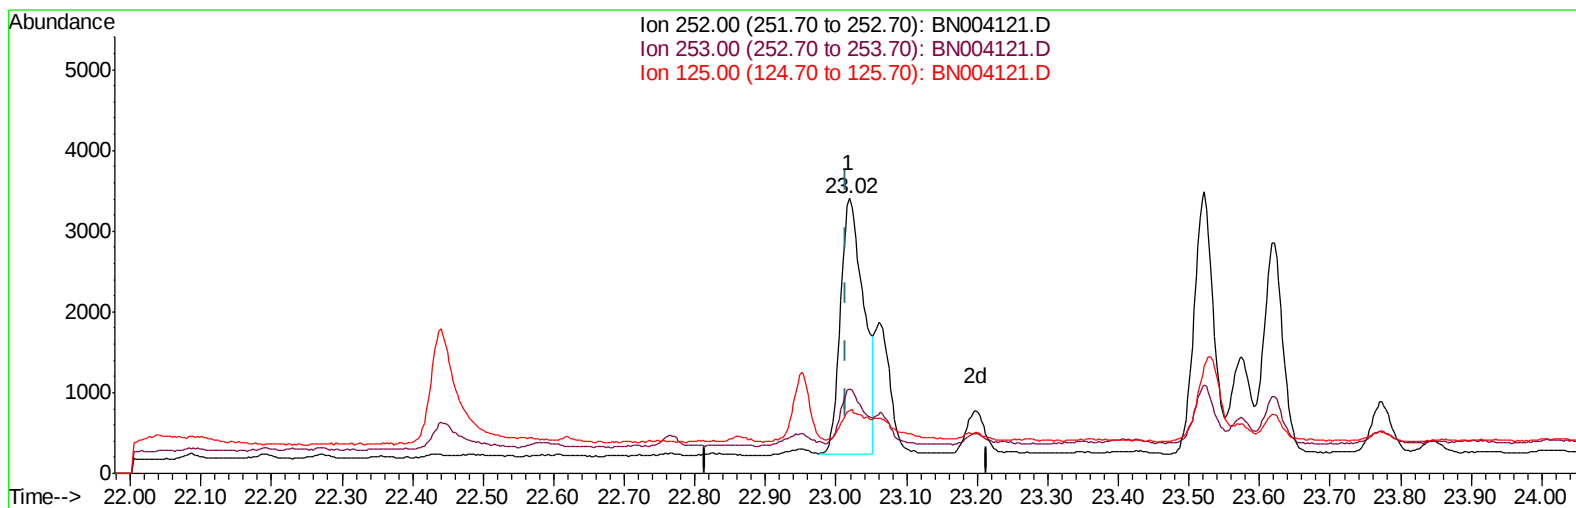

TIC: BN004121.D

(21) Benzo(b)fluoranthene

23.019min (+0.004) 0.15ng/ul m

response 7157

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 23.00 | 30.75  |
| 125.00 | 11.20 | 22.62# |
| 0.00   | 0.00  | 0.00   |