
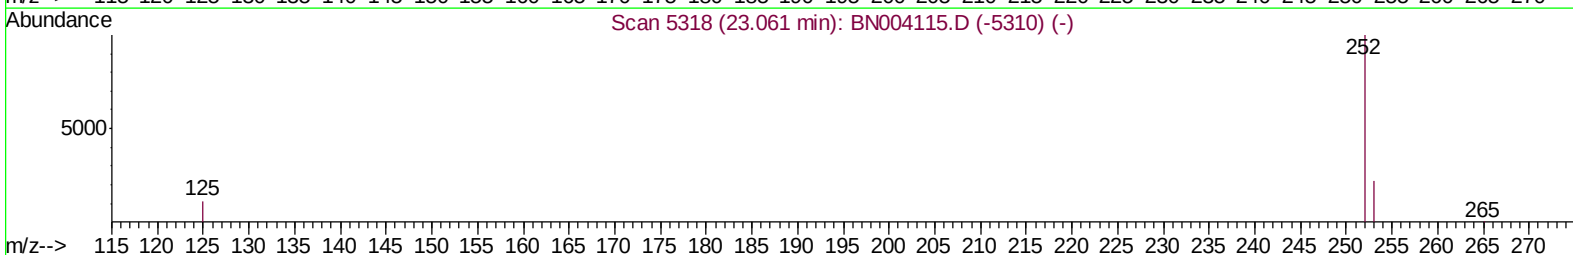
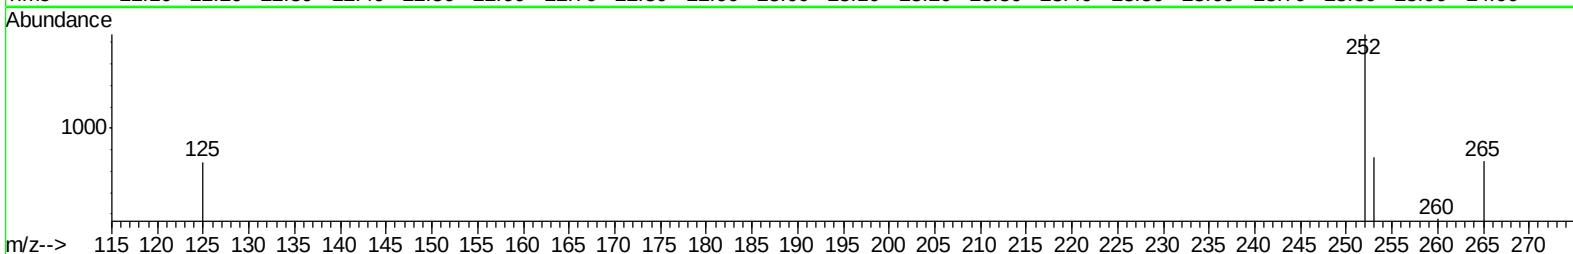


Data File : BN004121.D
Acq On : 19 Dec 2018 19:39
Operator : JU/SJ
Sample : J6297-11
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Dec 20 06:17:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 05:49:27 2018
Response via : Initial Calibration

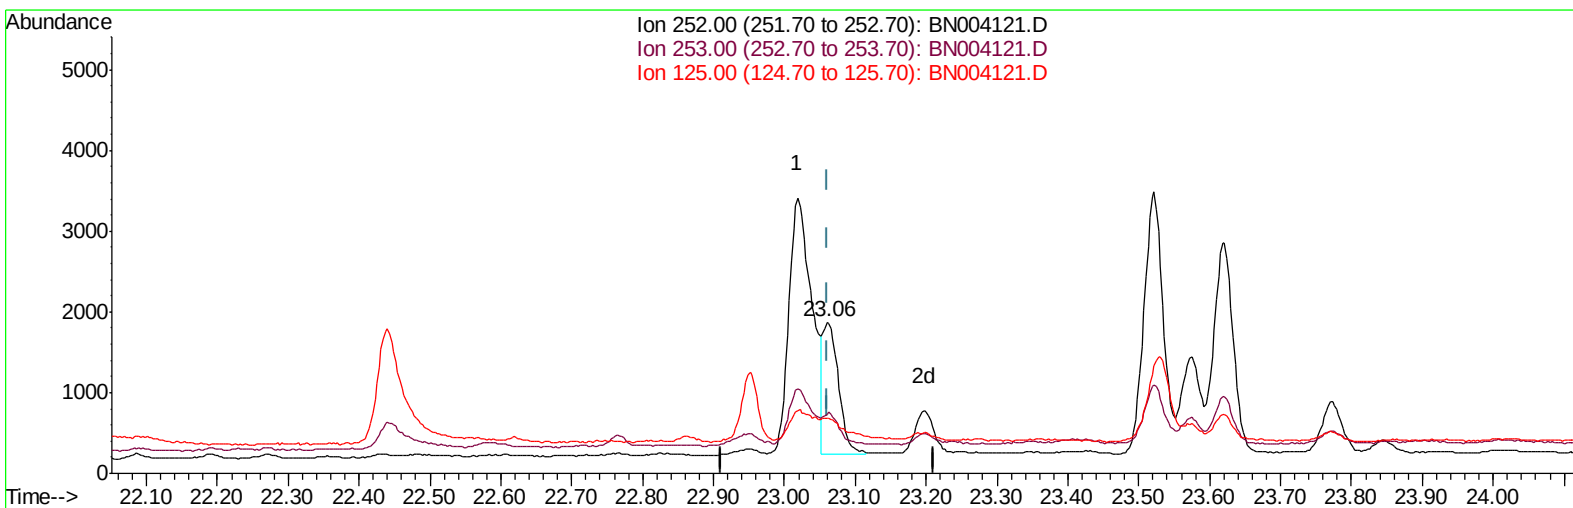

TIC: BN004121.D

(22) Benzo(k)fluoranthene

23.060min (-0.001) 0.06ng/ul m

response 2514

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	38.68#
125.00	11.30	36.60#
0.00	0.00	0.00