
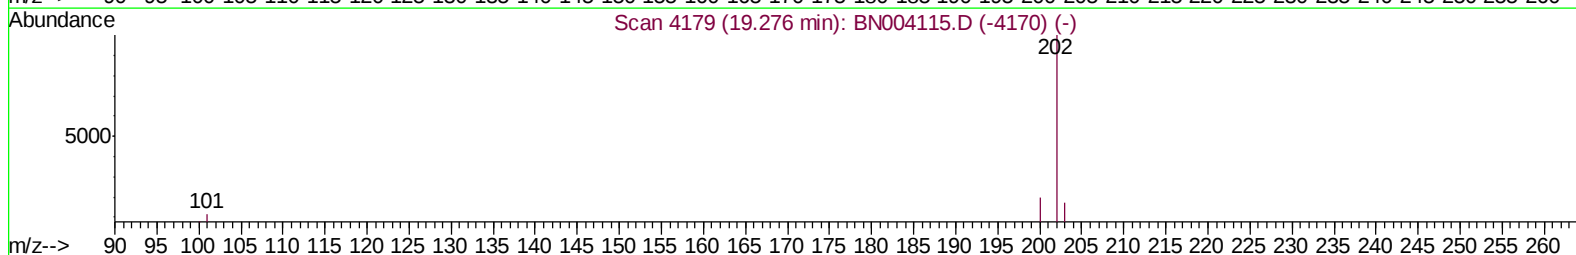
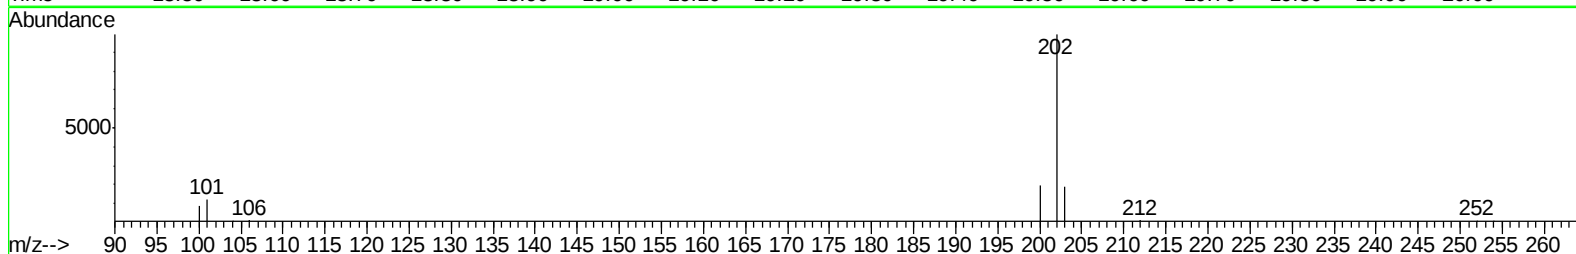


Data File : BN004124.D
Acq On : 19 Dec 2018 21:24
Operator : JU/SJ
Sample : J6297-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Dec 20 06:27:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 05:49:27 2018
Response via : Initial Calibration

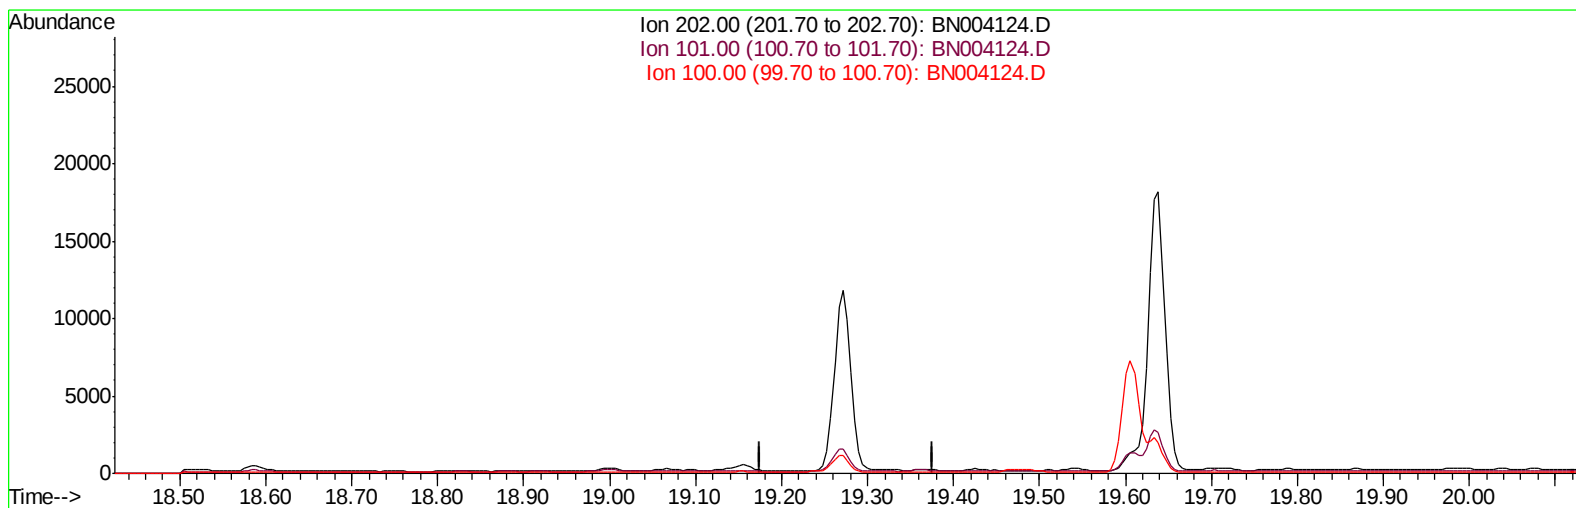

TIC: BN004124.D

(15) Fluoranthene (C)

19.276min (-19.276) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	10.70	0.00
100.00	8.10	0.00
0.00	0.00	0.00