
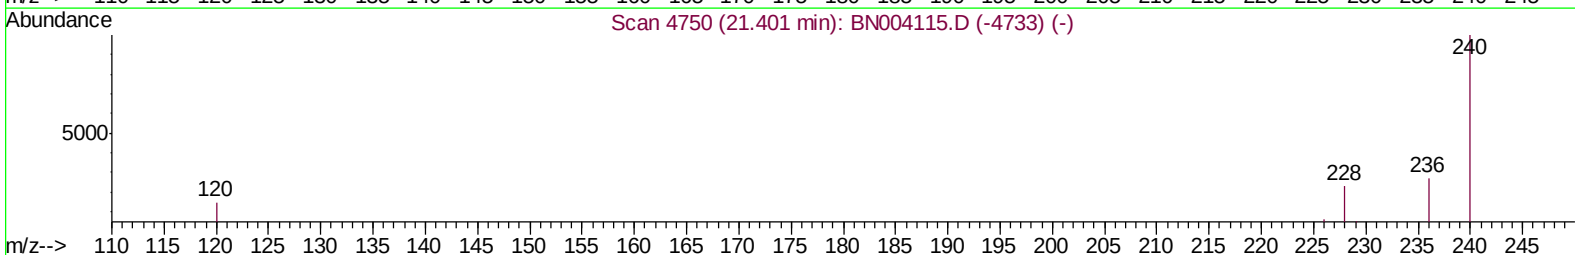
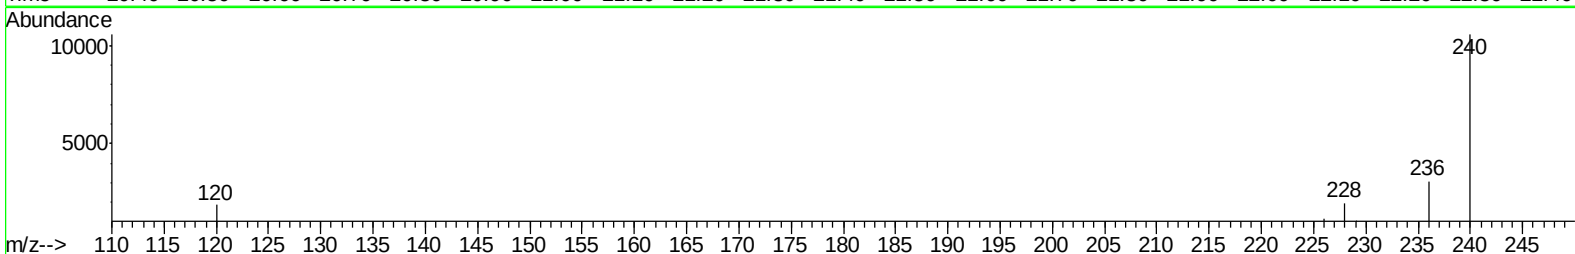


Data File : BN004124.D
Acq On : 19 Dec 2018 21:24
Operator : JU/SJ
Sample : J6297-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Dec 20 06:27:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 05:49:27 2018
Response via : Initial Calibration

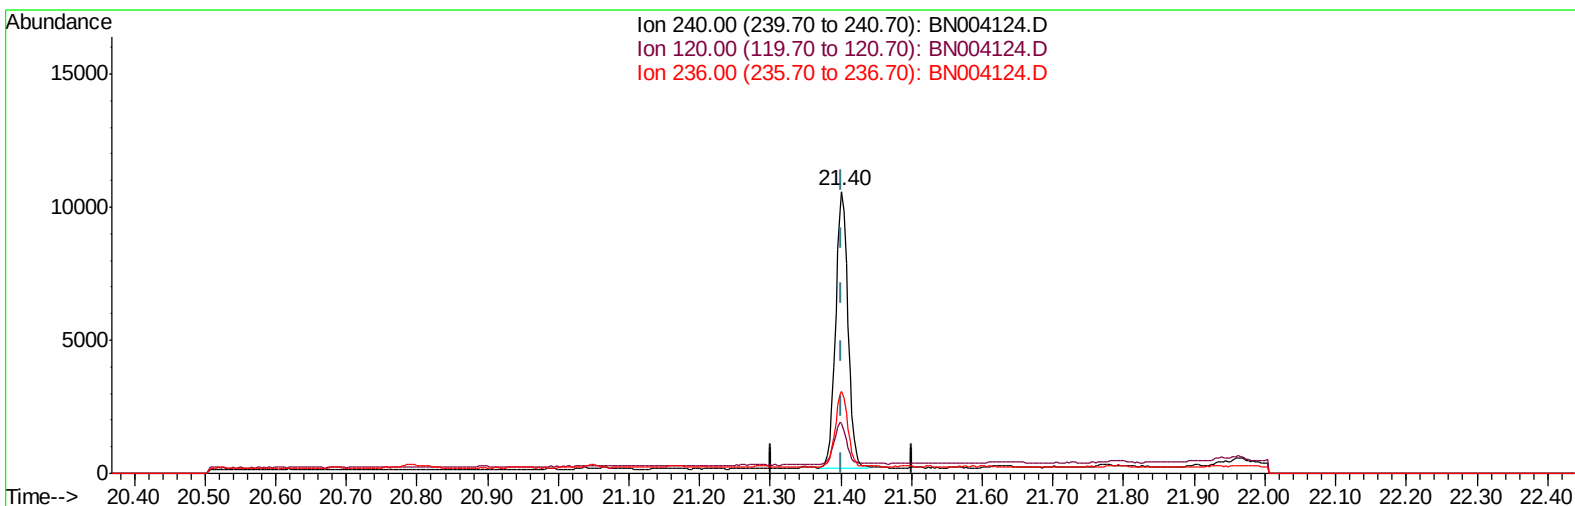

TIC: BN004124.D

(16) Chrysene-d12 (I)

21.401min (+0.000) 0.40ng/ul m

response 12719

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	17.68#
236.00	27.60	29.13
0.00	0.00	0.00