
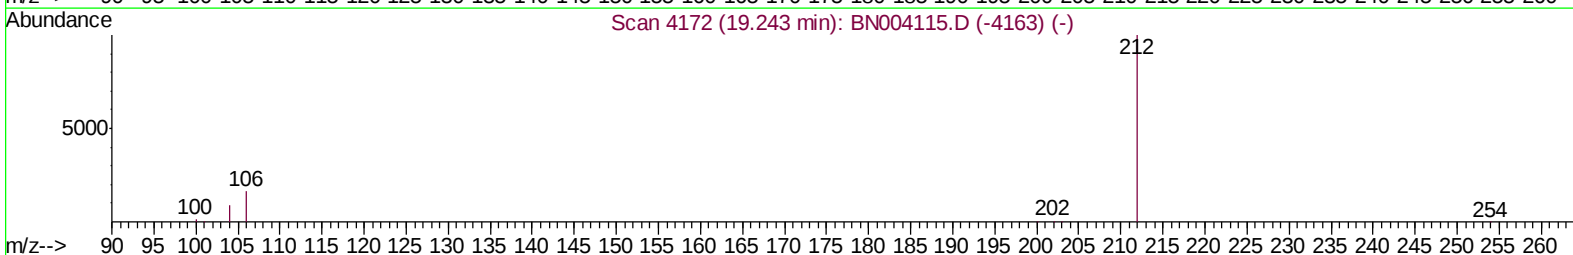
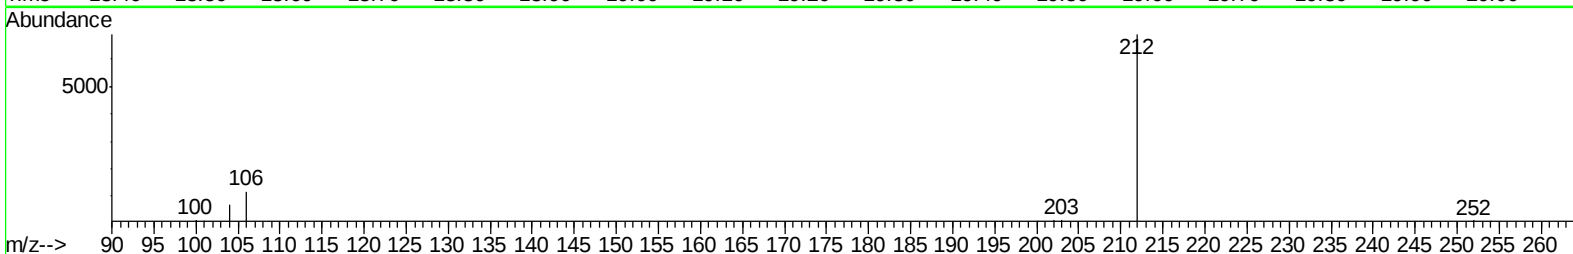


Data File : BN004125.D
Acq On : 19 Dec 2018 21:59
Operator : JU/SJ
Sample : PB115526BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Dec 20 06:33:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 05:49:27 2018
Response via : Initial Calibration

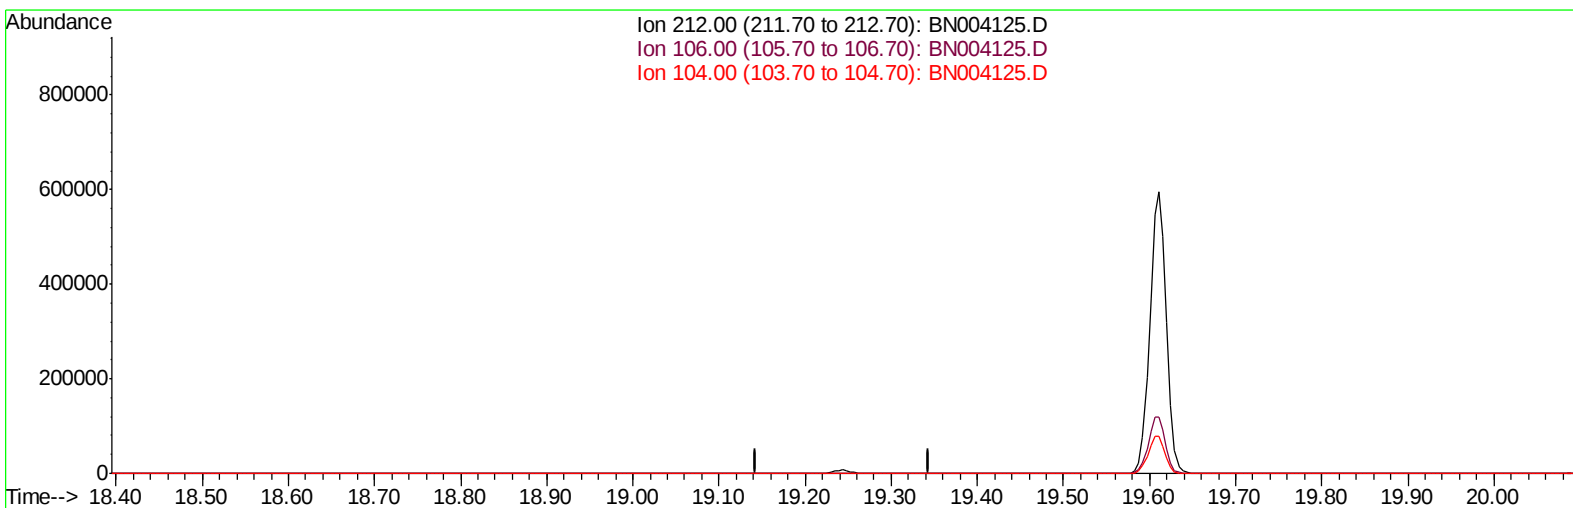

TIC: BN004125.D

(14) Fluoranthene-d10 (SURR)

19.243min (-19.243) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00