
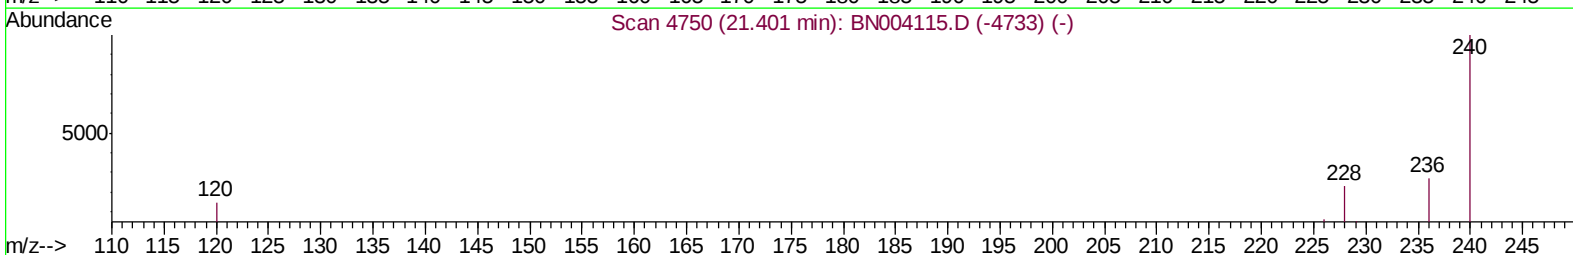
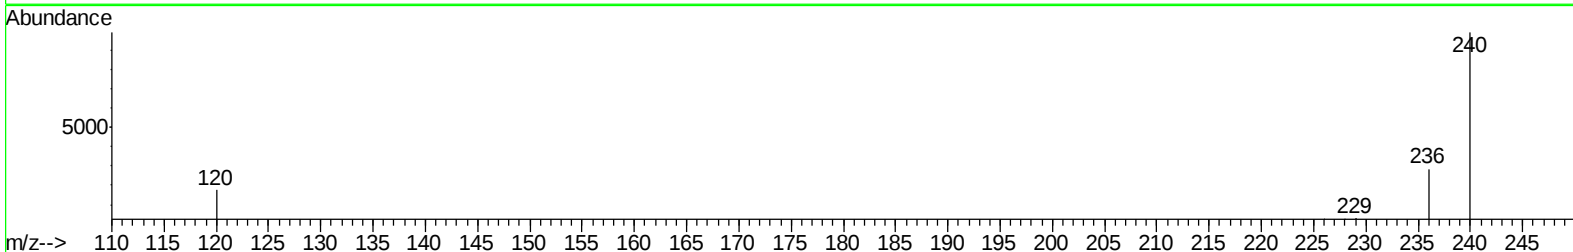


Data File : BN004125.D
Acq On : 19 Dec 2018 21:59
Operator : JU/SJ
Sample : PB115526BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Dec 20 06:33:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 05:49:27 2018
Response via : Initial Calibration

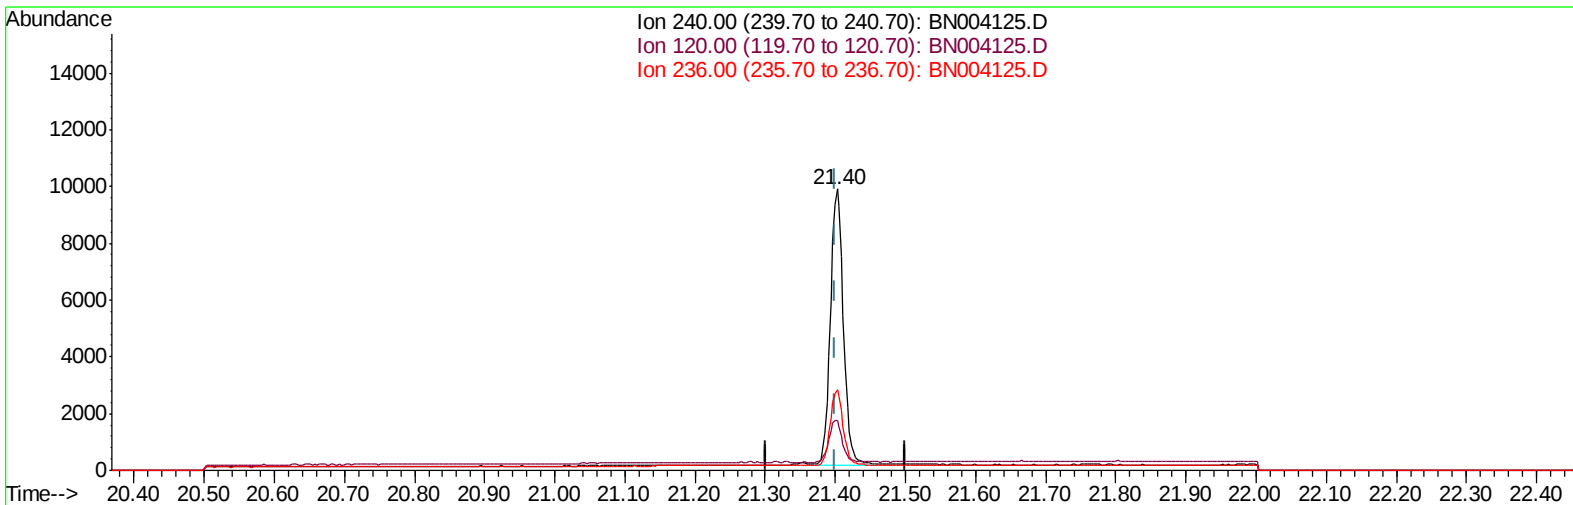

TIC: BN004125.D

(16) Chrysene-d12 (I)

21.403min (+0.001) 0.40ng/ul m

response 12427

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	17.72#
236.00	27.60	28.62
0.00	0.00	0.00