
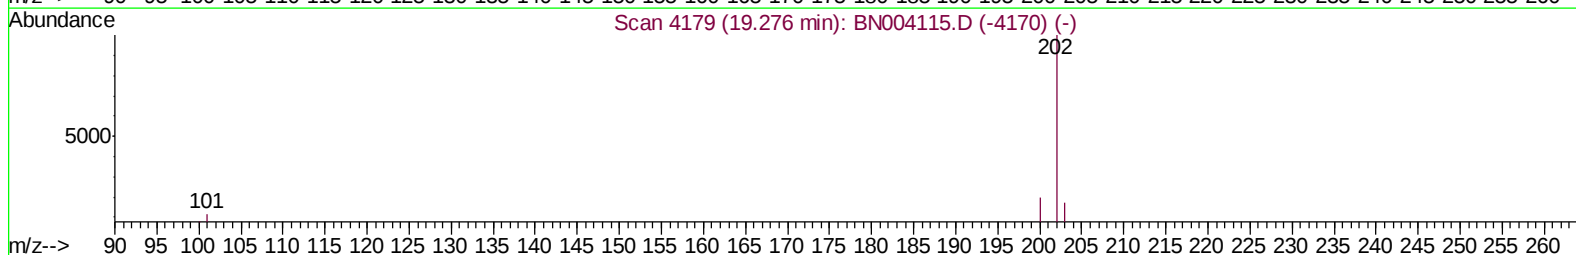
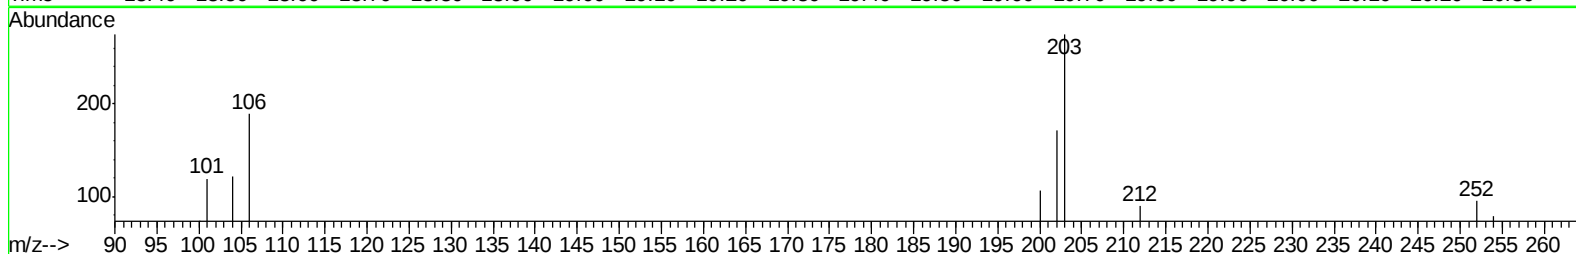


Data File : BN004126.D
Acq On : 19 Dec 2018 22:34
Operator : JU/SJ
Sample : J6299-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Dec 20 06:51:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 05:49:27 2018
Response via : Initial Calibration

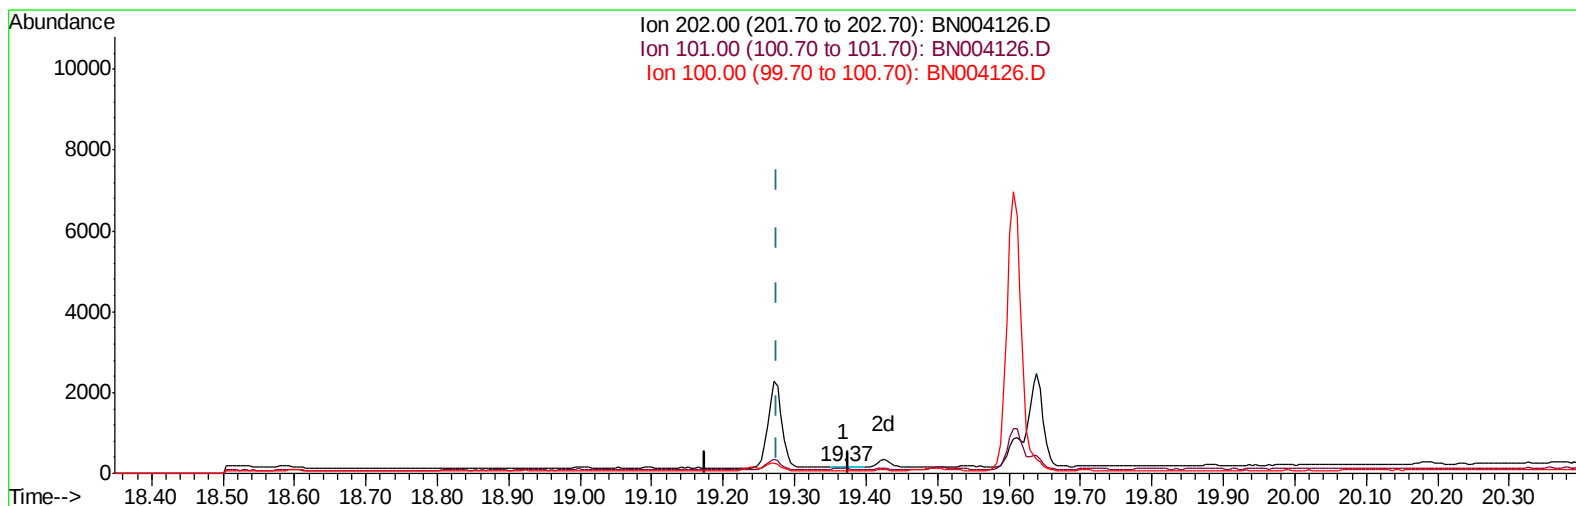

TIC: BN004126.D

(15) Fluoranthene (C)

19.369min (+0.093) 0.00ng/ul

response 33

Ion	Exp%	Act%
202.00	100	100
101.00	10.70	69.59#
100.00	8.10	42.69#
0.00	0.00	0.00