
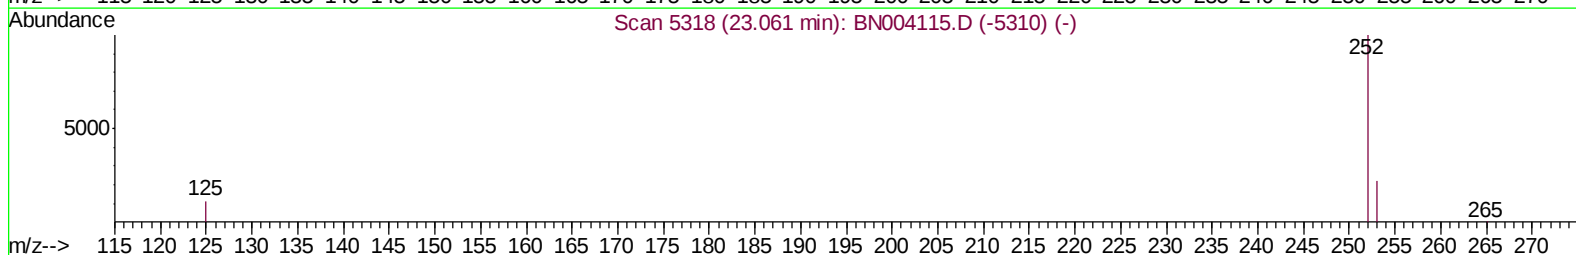
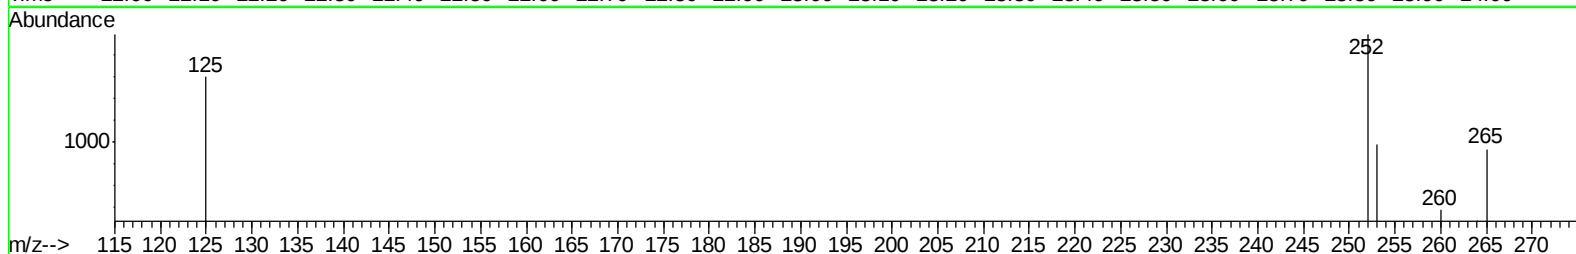


Data File : BN004126.D
Acq On : 19 Dec 2018 22:34
Operator : JU/SJ
Sample : J6299-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Dec 20 06:54:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 05:49:27 2018
Response via : Initial Calibration

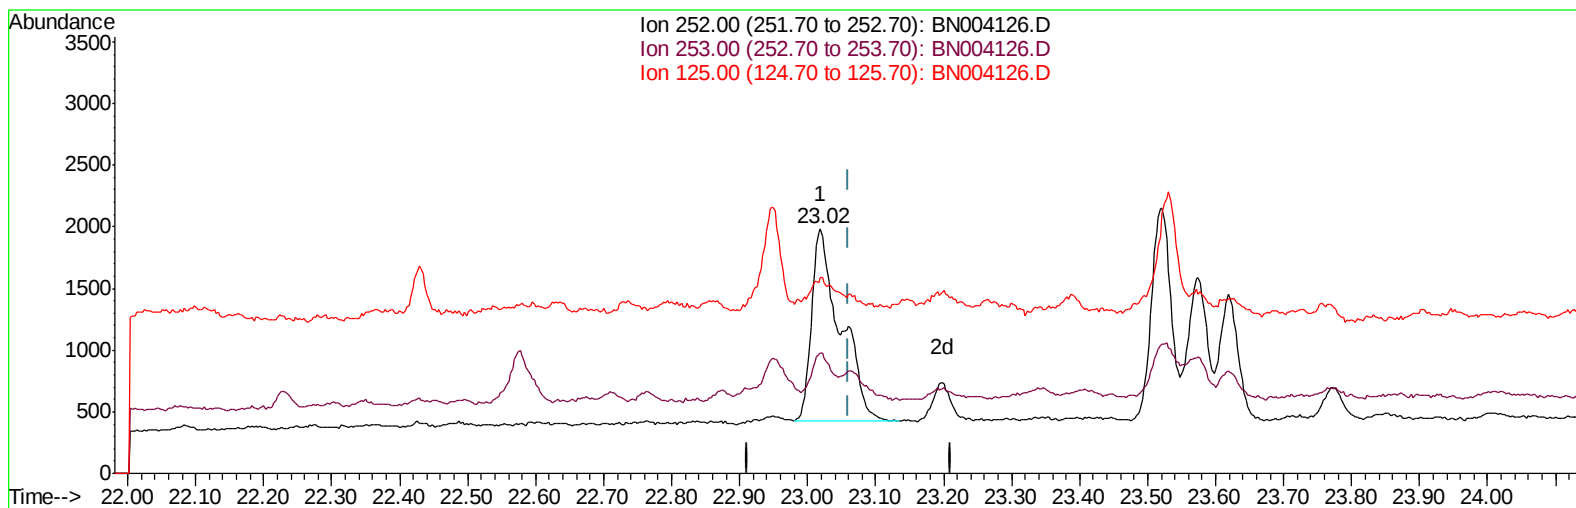

TIC: BN004126.D

(22) Benzo(k)fluoranthene
23.019min (-0.042) 0.09ng/ul
response 4616
Ion Exp% Act%
252.00 100 100
253.00 23.10 49.34#
125.00 11.30 80.29#
0.00 0.00 0.00