
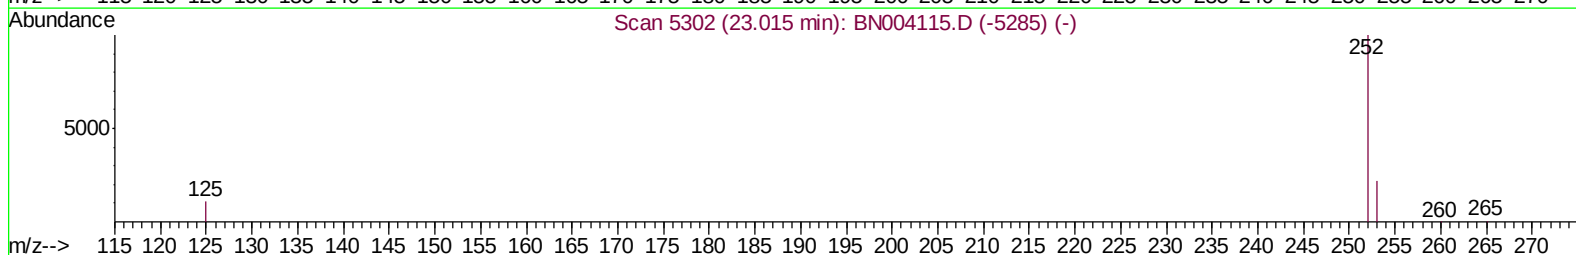
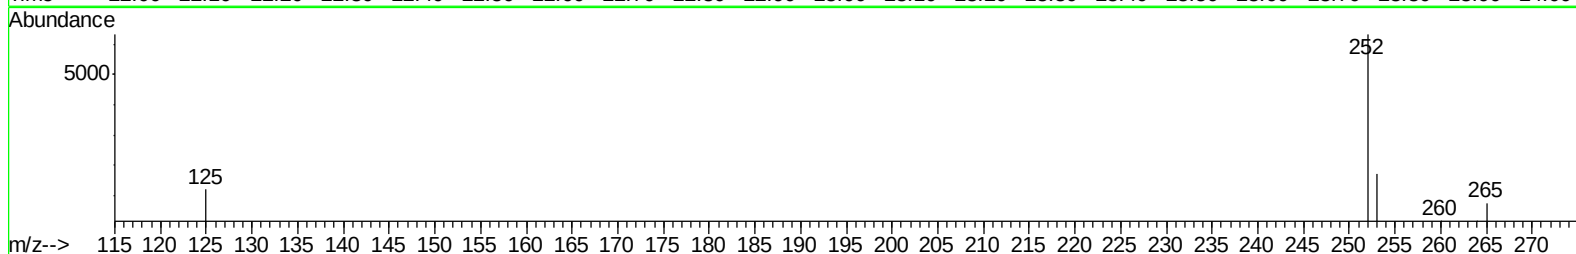


Data File : BN004128.D
Acq On : 19 Dec 2018 23:45
Operator : JU/SJ
Sample : J6299-03
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Dec 20 06:59:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 05:49:27 2018
Response via : Initial Calibration

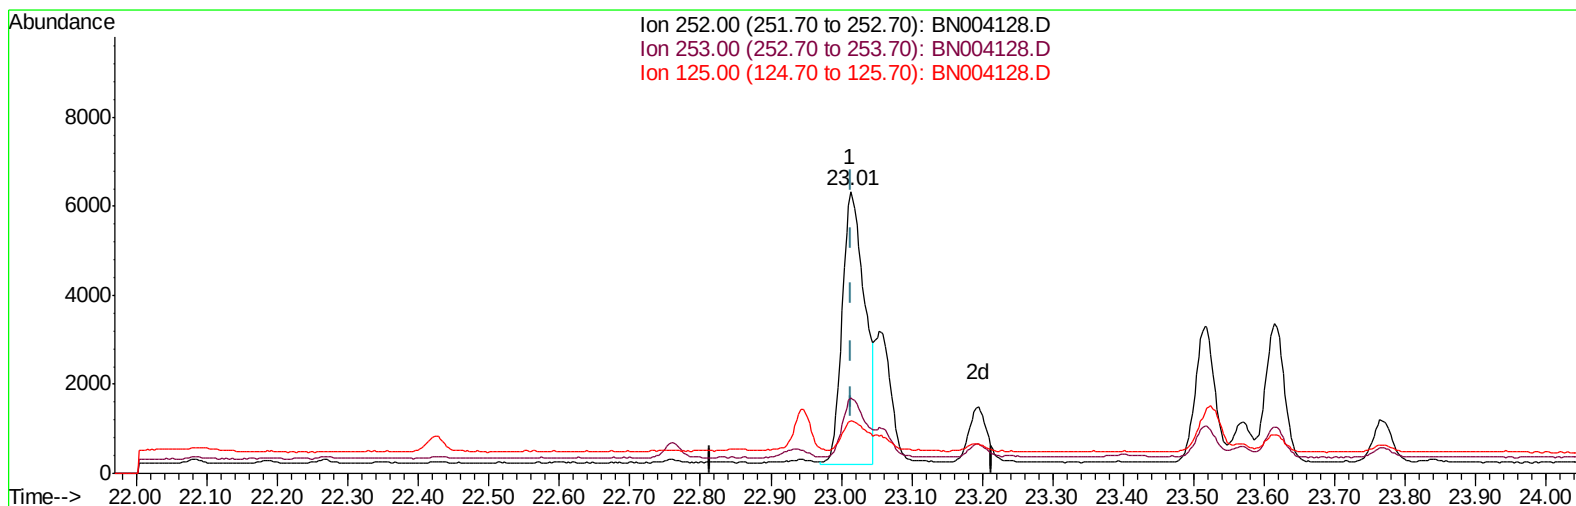

TIC: BN004128.D

(21) Benzo(b)fluoranthene

23.013min (-0.002) 0.28ng/ul m

response 13686

Ion	Exp%	Act%
252.00	100	100
253.00	23.00	26.98
125.00	11.20	18.84
0.00	0.00	0.00