
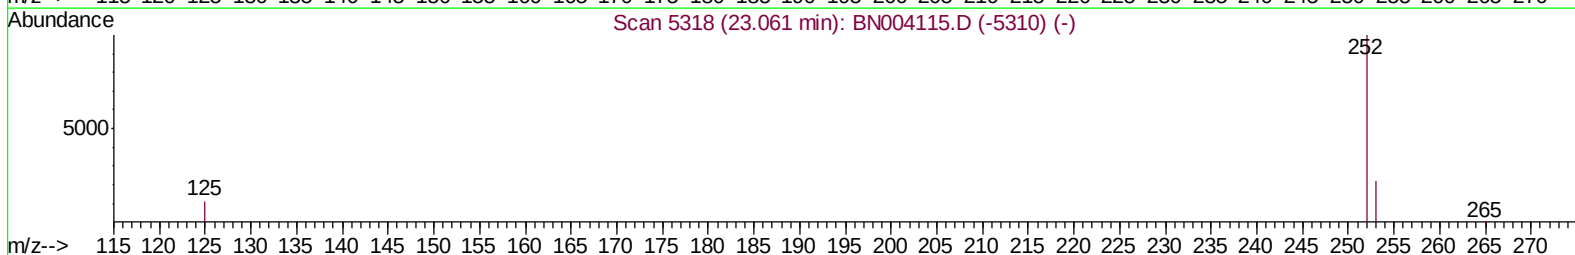
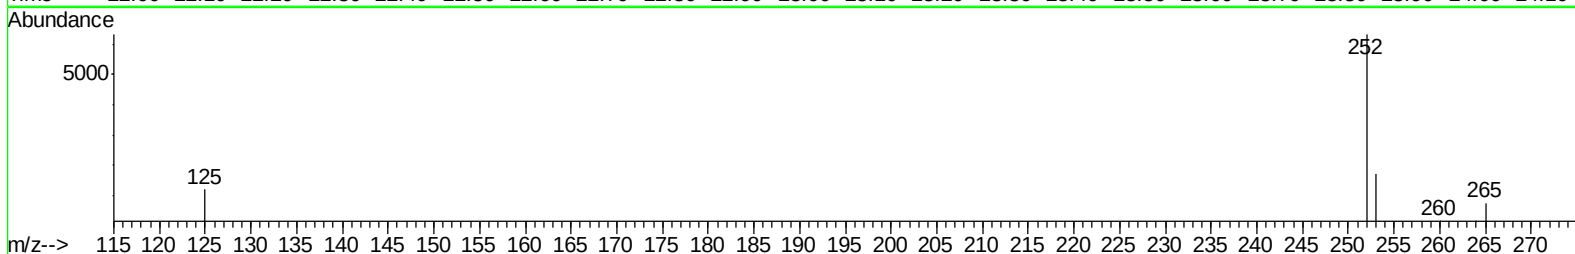


Data File : BN004128.D
Acq On : 19 Dec 2018 23:45
Operator : JU/SJ
Sample : J6299-03
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Dec 20 06:59:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 05:49:27 2018
Response via : Initial Calibration

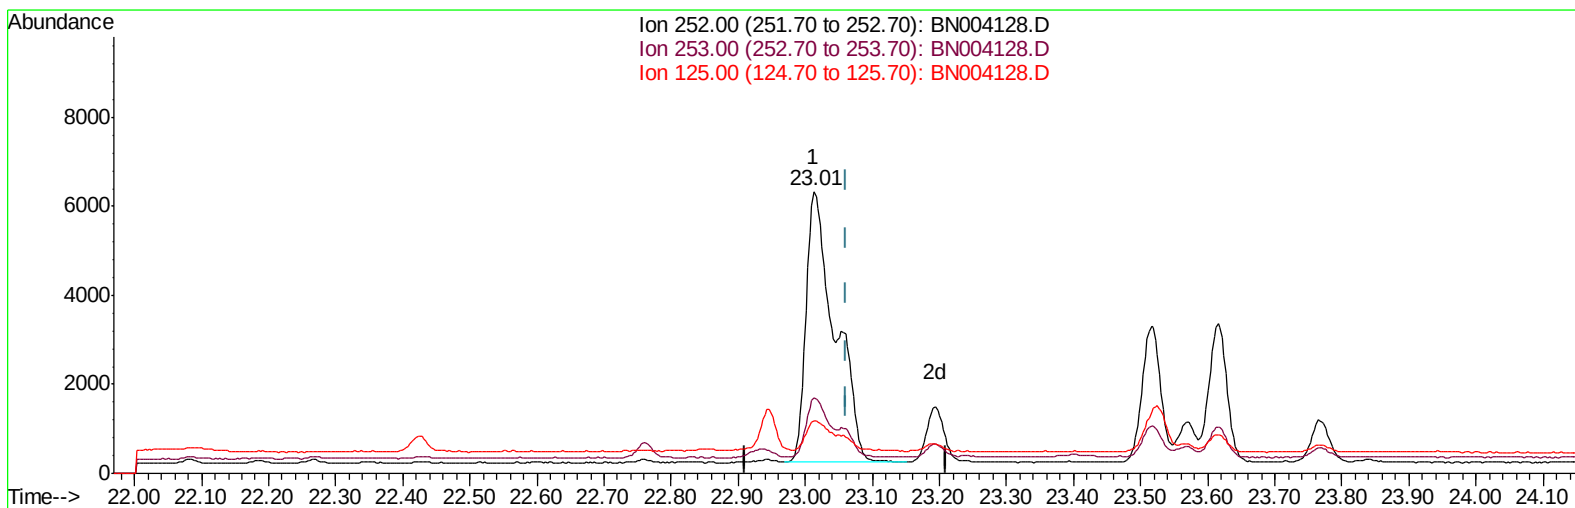

TIC: BN004128.D

(22) Benzo(k)fluoranthene
23.013min (-0.048) 0.38ng/ul
response 18065

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	26.98
125.00	11.30	18.84#
0.00	0.00	0.00