
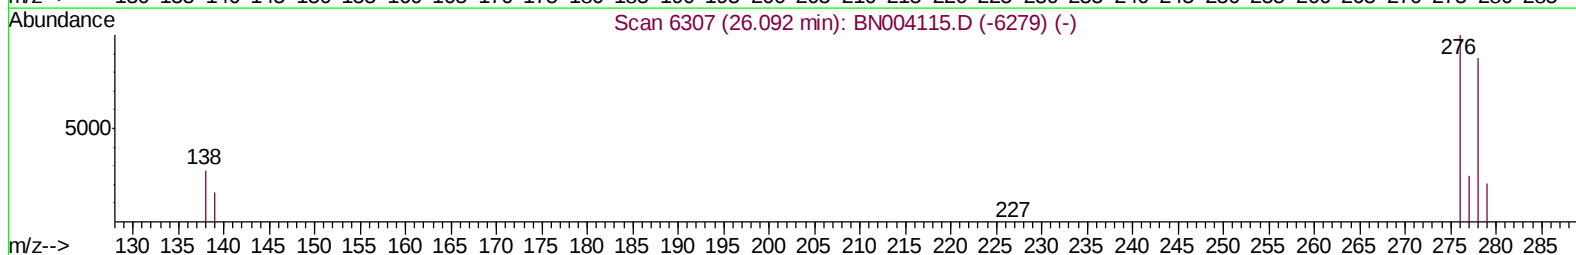
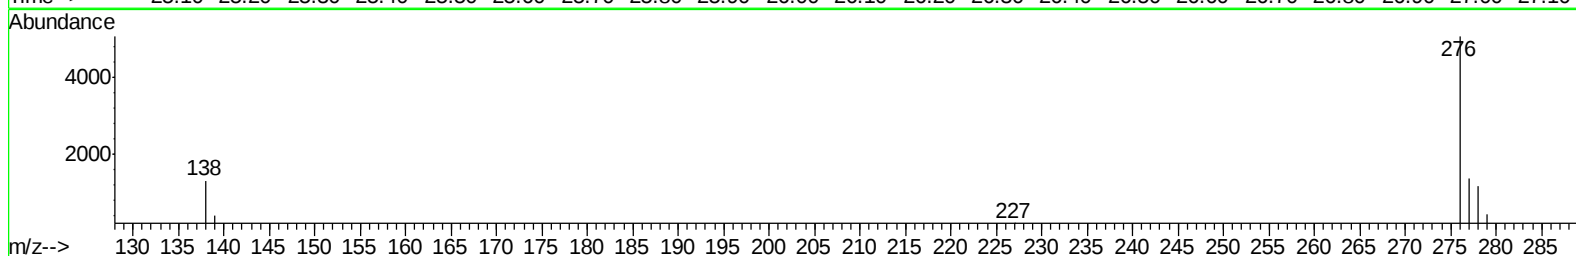


Data File : BN004129.D
Acq On : 20 Dec 2018 00:20
Operator : JU/SJ
Sample : J6299-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Dec 20 05:54:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 05:49:27 2018
Response via : Initial Calibration

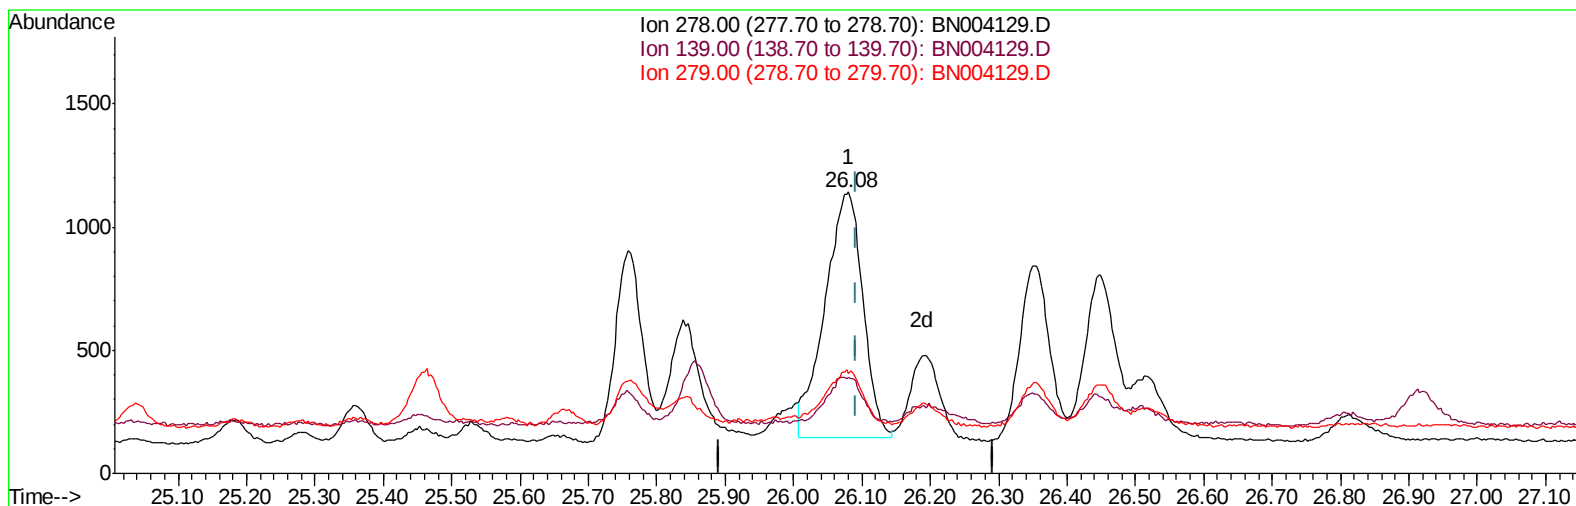

TIC: BN004129.D

(25) Dibenzo(a,h)anthracene

26.081min (-0.012) 0.09ng/ul m

response 3838

Ion	Exp%	Act%
278.00	100	100
139.00	17.80	34.21#
279.00	24.70	35.61#
0.00	0.00	0.00