
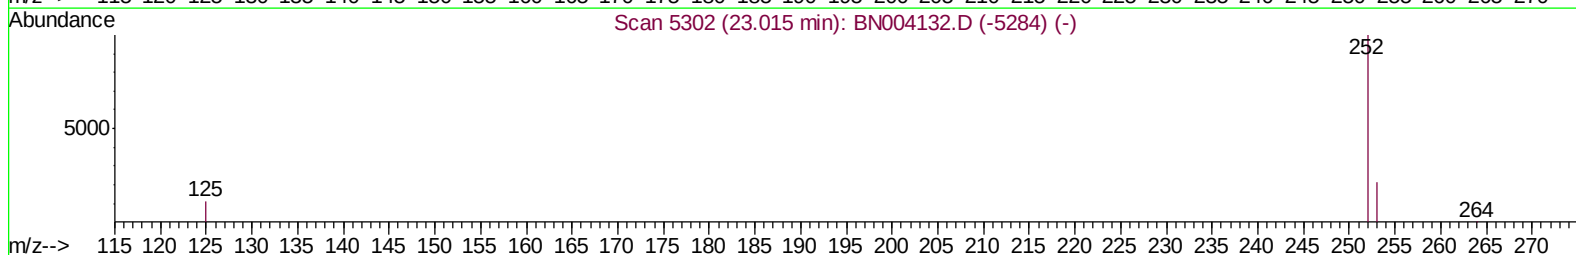
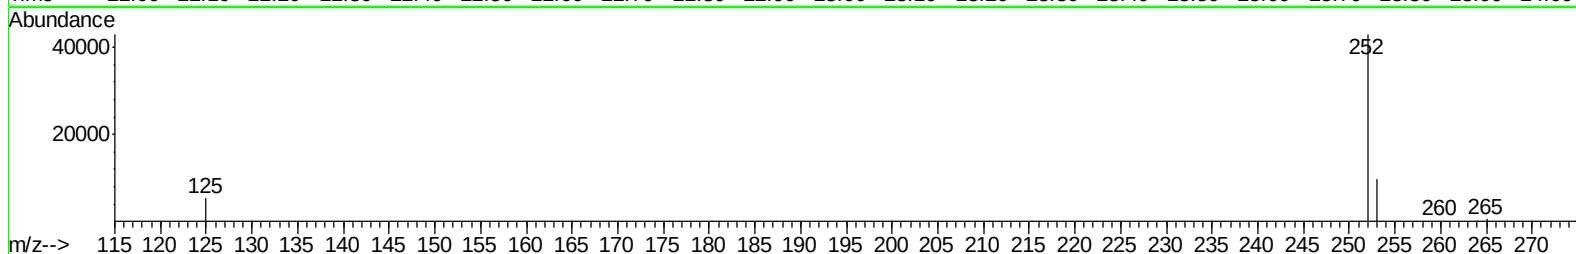


Data File : BN004134.D
Acq On : 20 Dec 2018 03:15
Operator : JU/SJ
Sample : J6299-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Quant Time: Dec 20 07:31:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

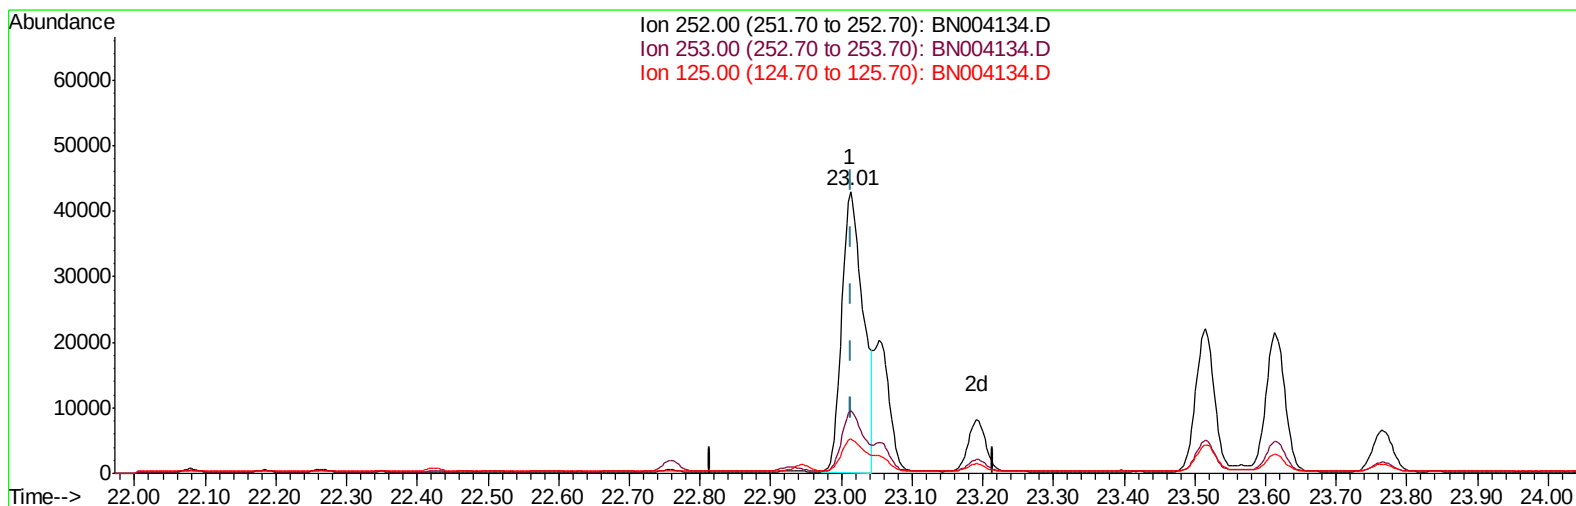

TIC: BN004134.D

(21) Benzo(b)fluoranthene

23.013min (-0.002) 1.75ng/ul m

response 89664

Ion	Exp%	Act%
252.00	100	100
253.00	23.00	22.51
125.00	11.20	12.43
0.00	0.00	0.00