
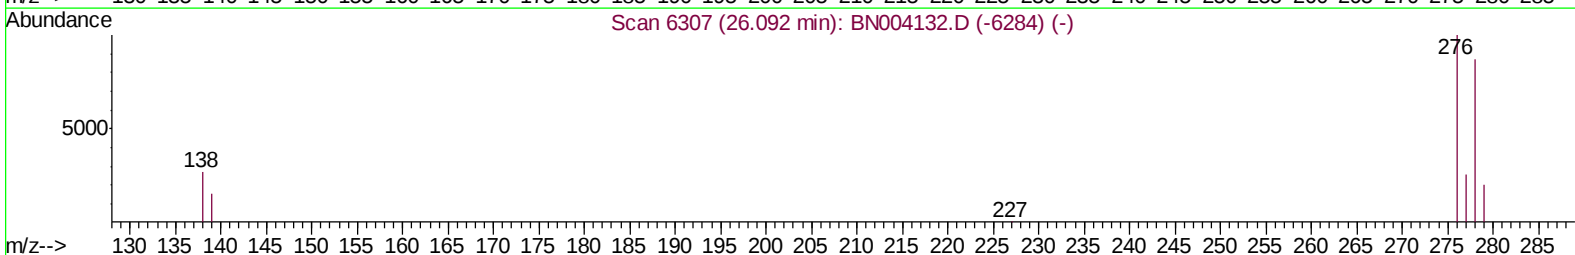
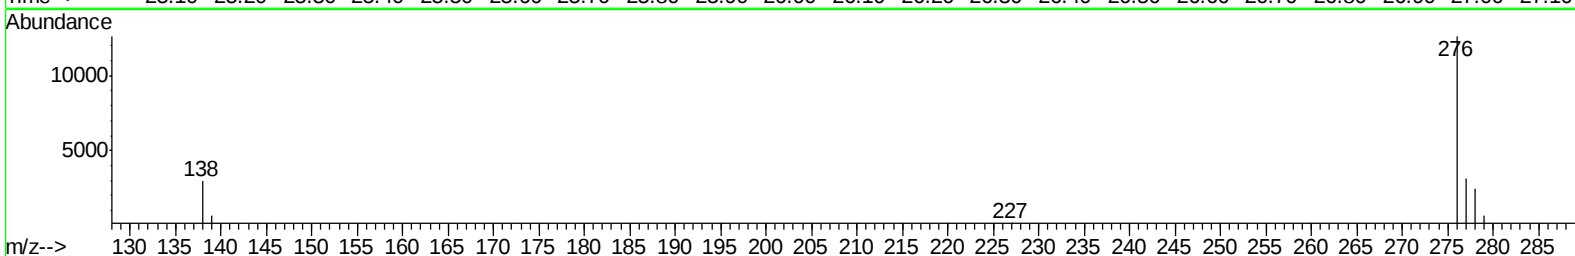


Data File : BN004134.D
Acq On : 20 Dec 2018 03:15
Operator : JU/SJ
Sample : J6299-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Quant Time: Dec 20 07:31:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

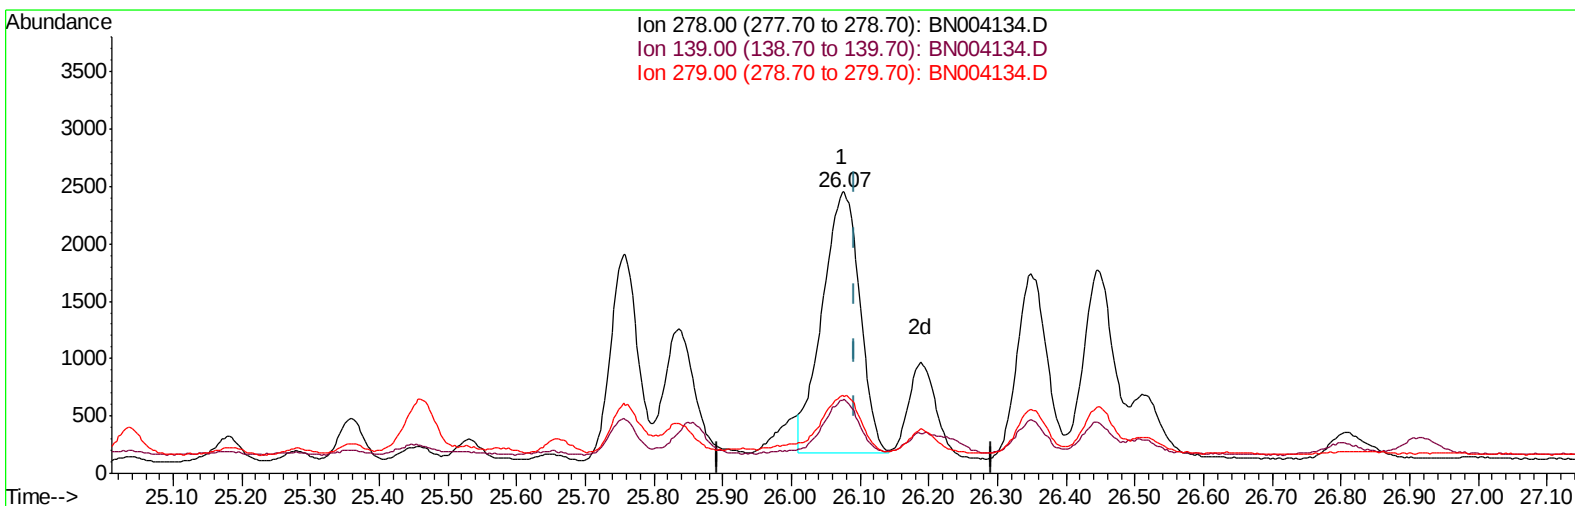

TIC: BN004134.D

(25) Dibenzo(a,h)anthracene

26.074min (-0.018) 0.21ng/ul m

response 8656

Ion	Exp%	Act%
278.00	100	100
139.00	17.80	26.04#
279.00	24.70	27.83
0.00	0.00	0.00