
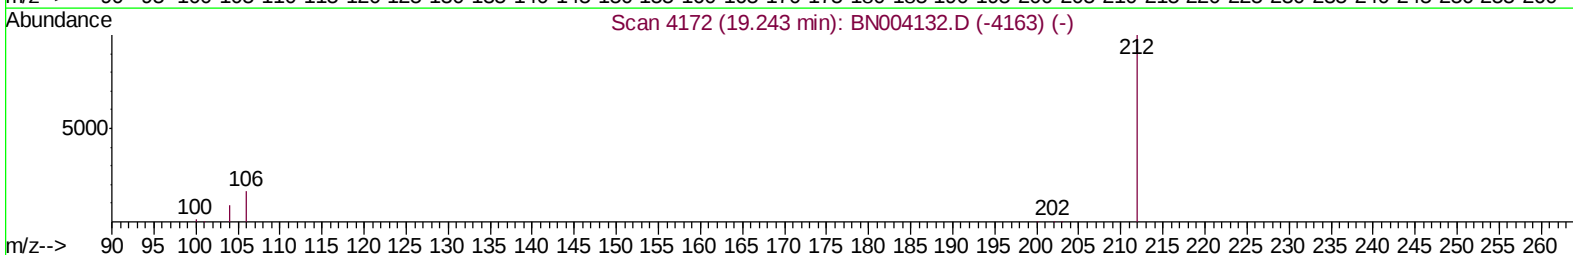
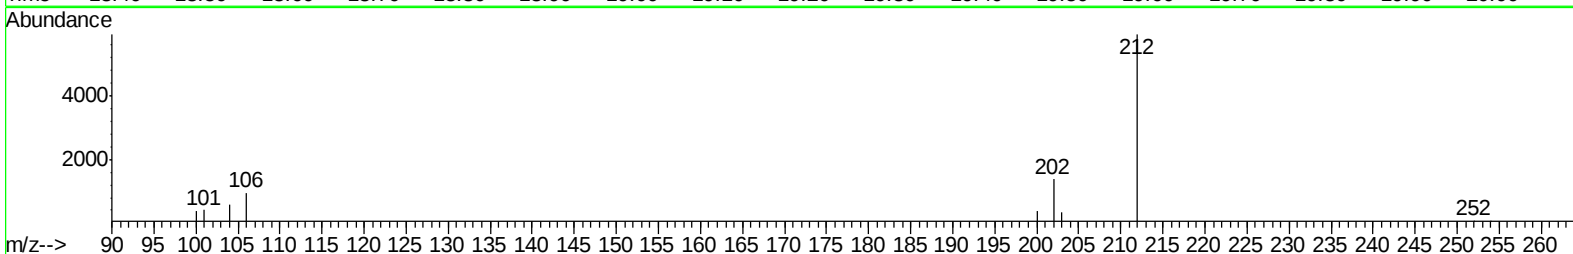


Data File : BN004135.D  
Acq On : 20 Dec 2018 03:50  
Operator : JU/SJ  
Sample : J6299-09  
Misc :  
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Dec 20 07:34:08 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-SIM-BN111918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Dec 20 07:15:48 2018  
Response via : Initial Calibration

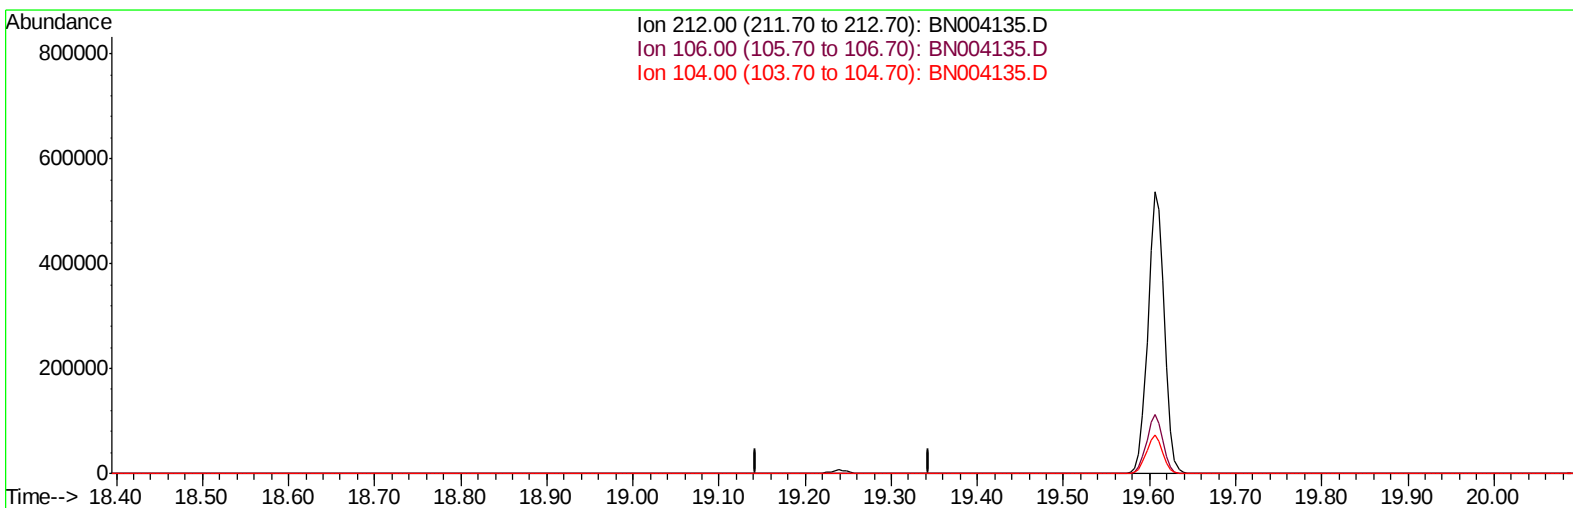

TIC: BN004135.D

(14) Fluoranthene-d10 (SURR)

19.243min (-19.243) 0.00ng/ul

response 0

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 212.00 | 100   | 0.00  |
| 106.00 | 14.20 | 0.00# |
| 104.00 | 8.00  | 0.00# |
| 0.00   | 0.00  | 0.00  |