
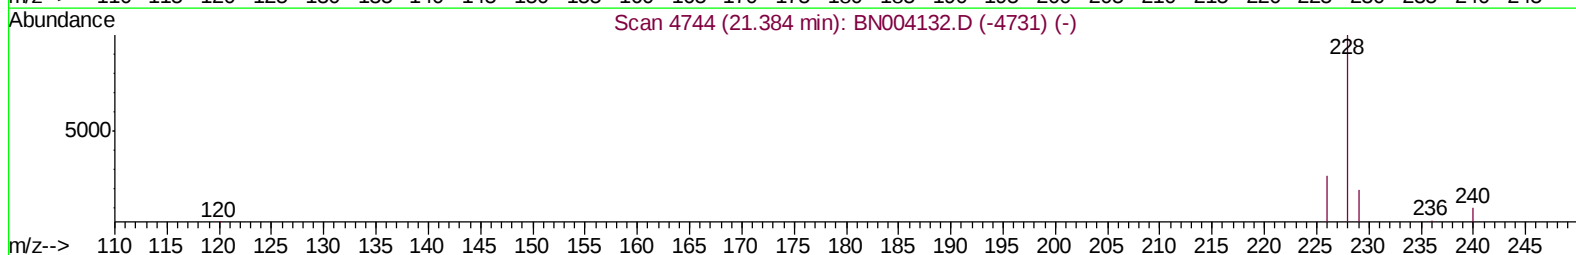
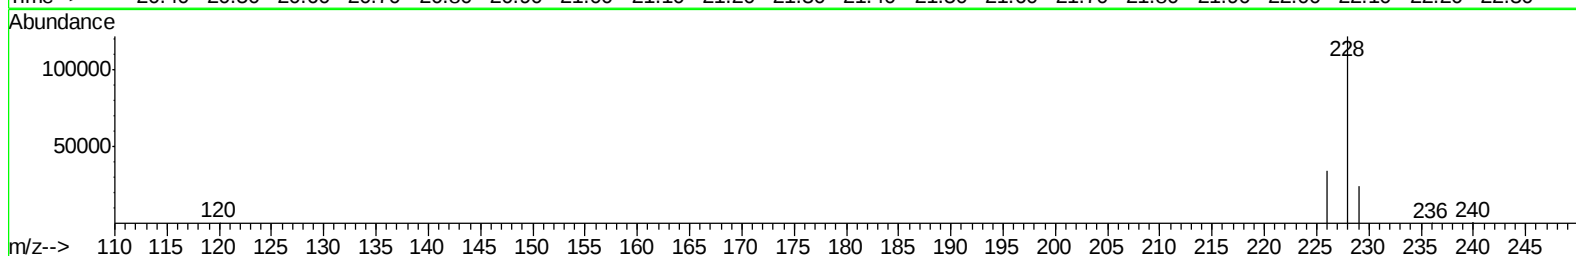


Data File : BN004135.D
Acq On : 20 Dec 2018 03:50
Operator : JU/SJ
Sample : J6299-09
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Dec 20 07:35:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

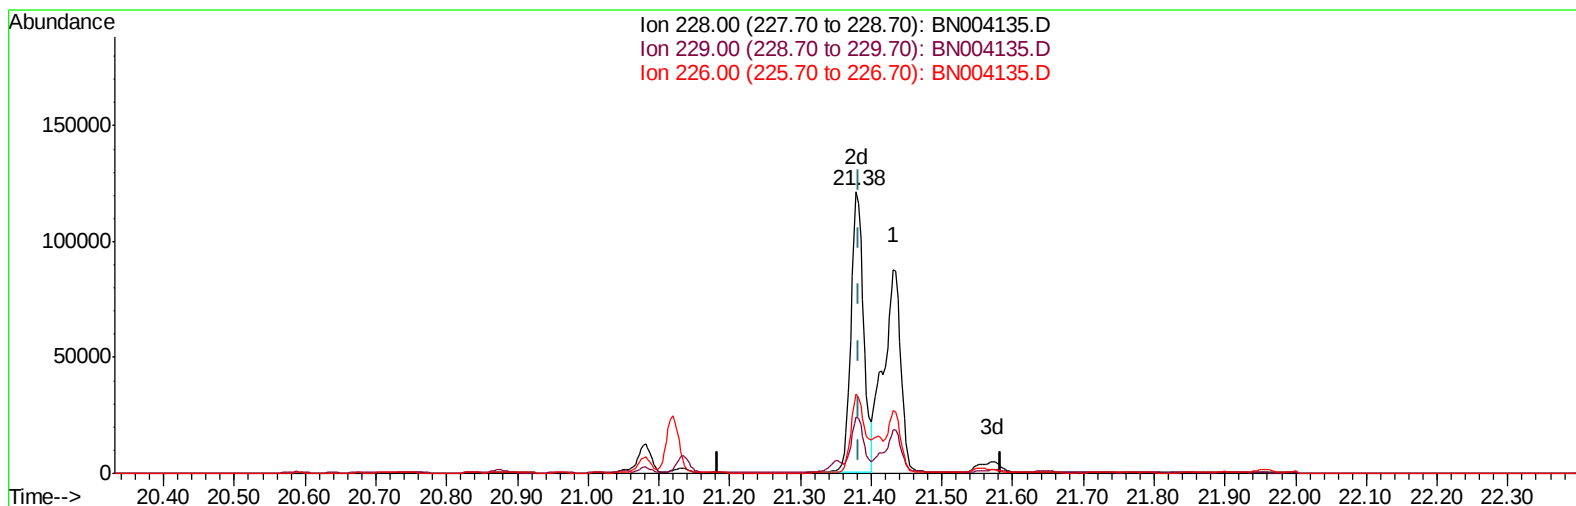

TIC: BN004135.D

(18) Benzo(a)anthracene
21.379min (-0.005) 3.77ng/ul m
response 151256

Ion	Exp%	Act%
228.00	100	100
229.00	19.50	20.02
226.00	26.40	28.06
0.00	0.00	0.00