
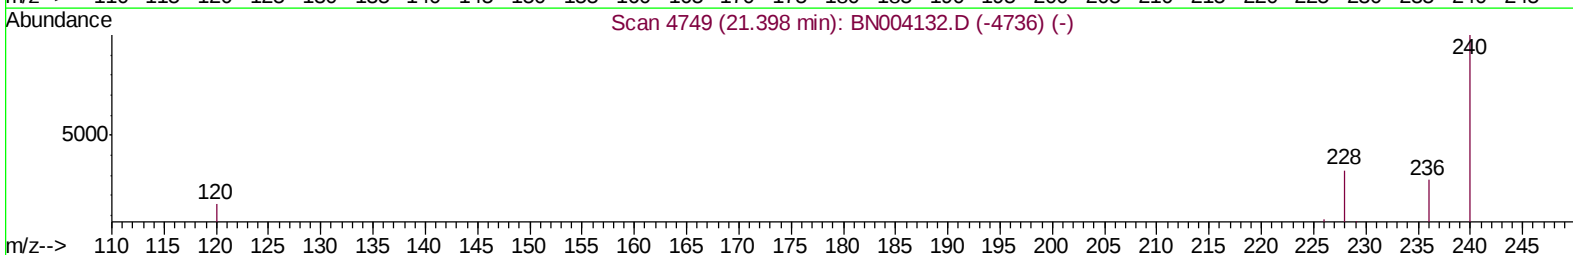
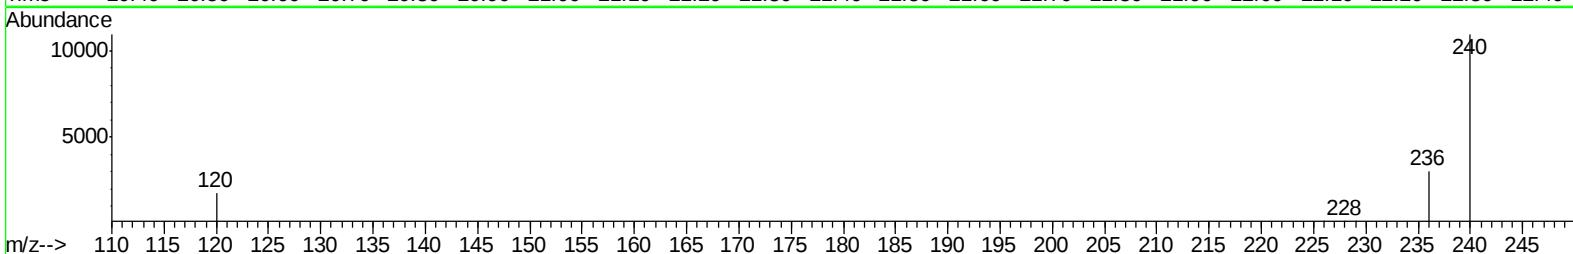


Data File : BN004137.D
Acq On : 20 Dec 2018 05:00
Operator : JU/SJ
Sample : J6299-11
Misc :
ALS Vial : 34 Sample Multiplier: 1

Quant Time: Dec 20 07:44:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

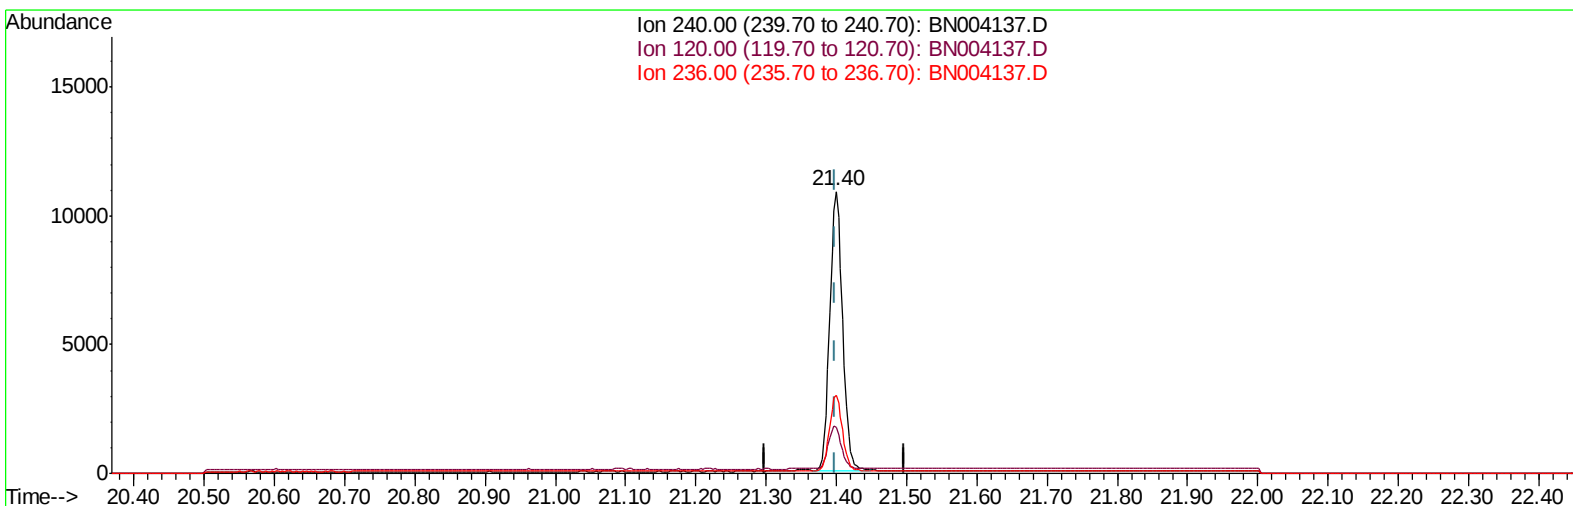

TIC: BN004137.D

(16) Chrysene-d12 (I)

21.400min (+0.001) 0.40ng/ul m

response 13484

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	16.35
236.00	27.60	27.79
0.00	0.00	0.00