
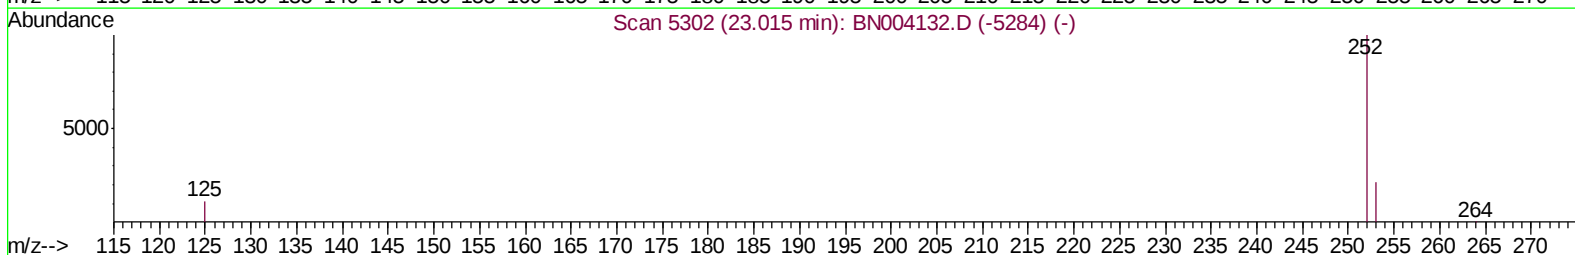
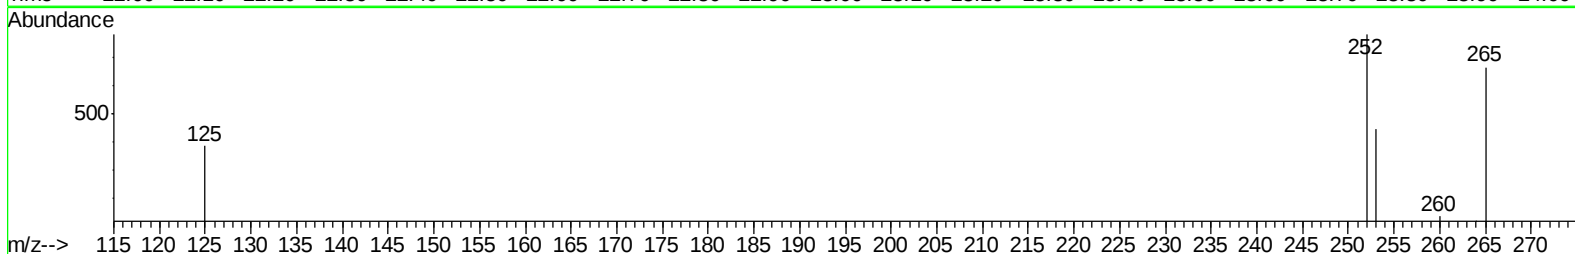


Data File : BN004139.D
Acq On : 20 Dec 2018 06:10
Operator : JU/SJ
Sample : J6297-16
Misc :
ALS Vial : 36 Sample Multiplier: 1

Quant Time: Dec 20 07:51:03 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

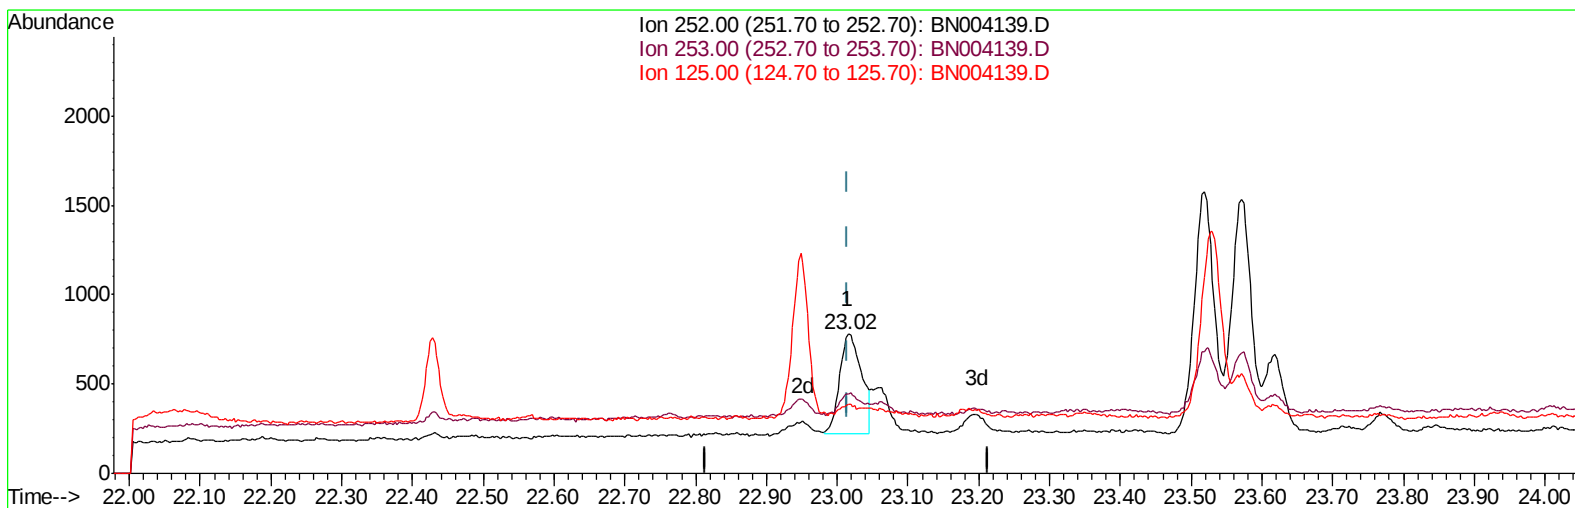

TIC: BN004139.D

(21) Benzo(b)fluoranthene

23.016min (+0.001) 0.02ng/ul m

response 1201

Ion	Exp%	Act%
252.00	100	100
253.00	23.00	57.18#
125.00	11.20	49.36#
0.00	0.00	0.00