
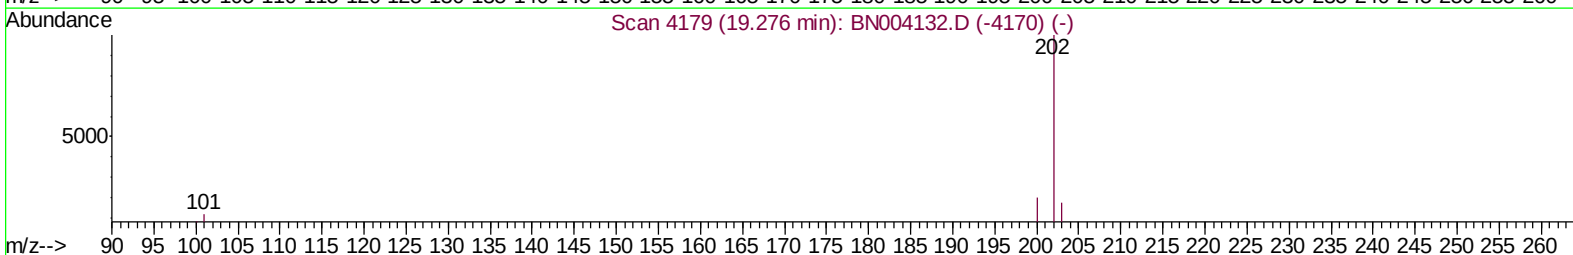
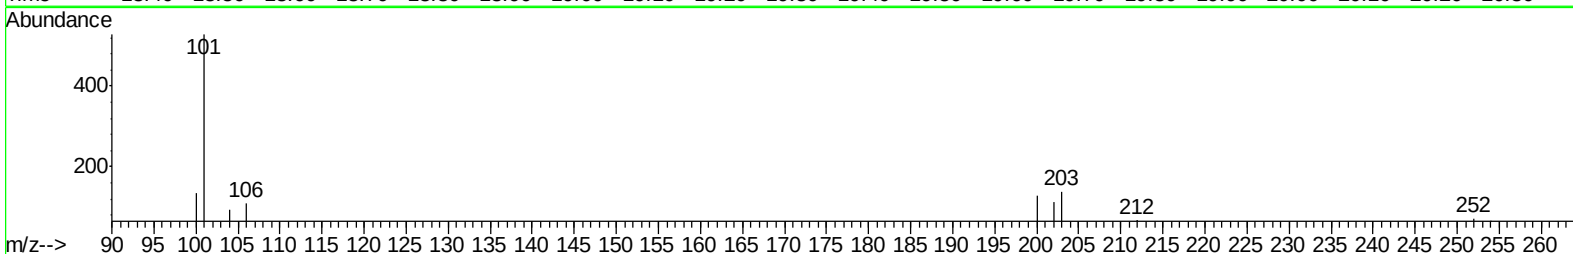


Data File : BN004140.D  
Acq On : 20 Dec 2018 06:45  
Operator : JU/SJ  
Sample : J6297-17  
Misc :  
ALS Vial : 37 Sample Multiplier: 1

Quant Time: Dec 20 07:52:34 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-SIM-BN111918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Dec 20 07:15:48 2018  
Response via : Initial Calibration

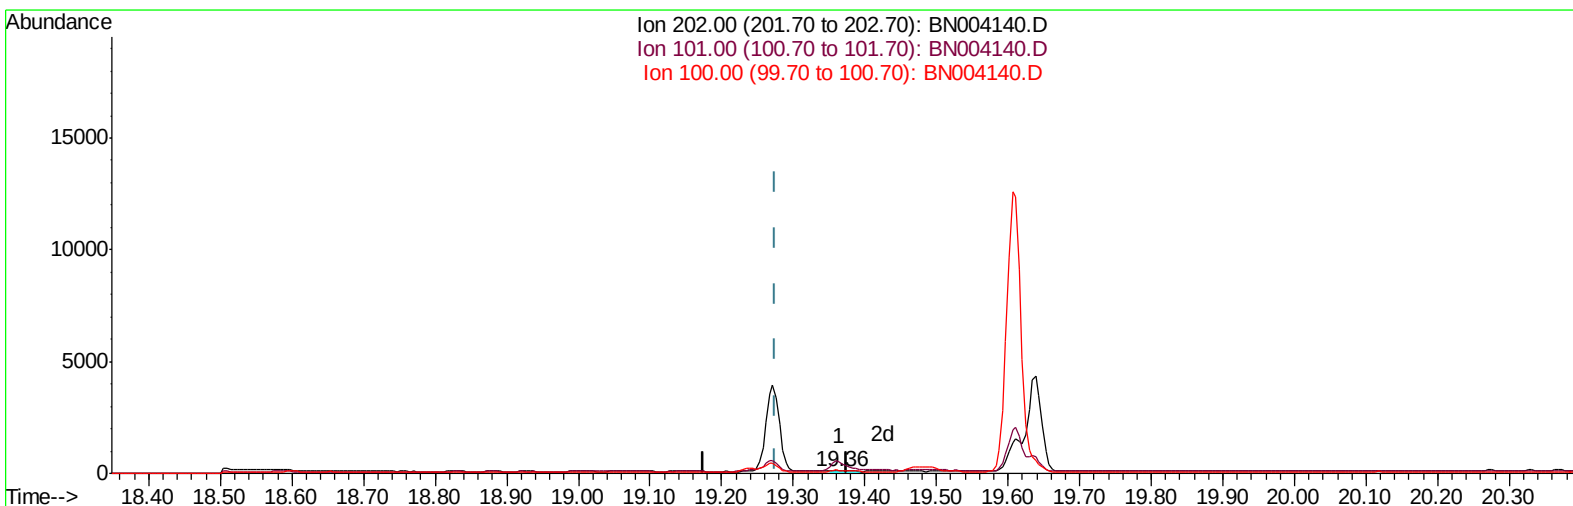

TIC: BN004140.D

(15) Fluoranthene (C)

19.364min (+0.089) 0.00ng/ul

response 44

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 202.00 | 100   | 100     |
| 101.00 | 10.70 | 463.16# |
| 100.00 | 8.10  | 119.30# |
| 0.00   | 0.00  | 0.00    |