

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Not Reviewed)

Data File : BN004111.D
Acq On : 19 Dec 2018 13:46
Operator : JU/SJ
Sample : J6297-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E39

Quant Time: Dec 20 04:45:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 04:42:11 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	889	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	4688	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	3163	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	643354	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.72	264	12148	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	2196	0.30	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.57	252	3141	0.072	ng/ul#	Qvalue 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN004111.D
Acq On : 19 Dec 2018 13:46
Operator : JU/SJ
Sample : J6297-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E39

Quant Time: Dec 20 04:45:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN11918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 04:42:11 2018
Response via : Initial Calibration

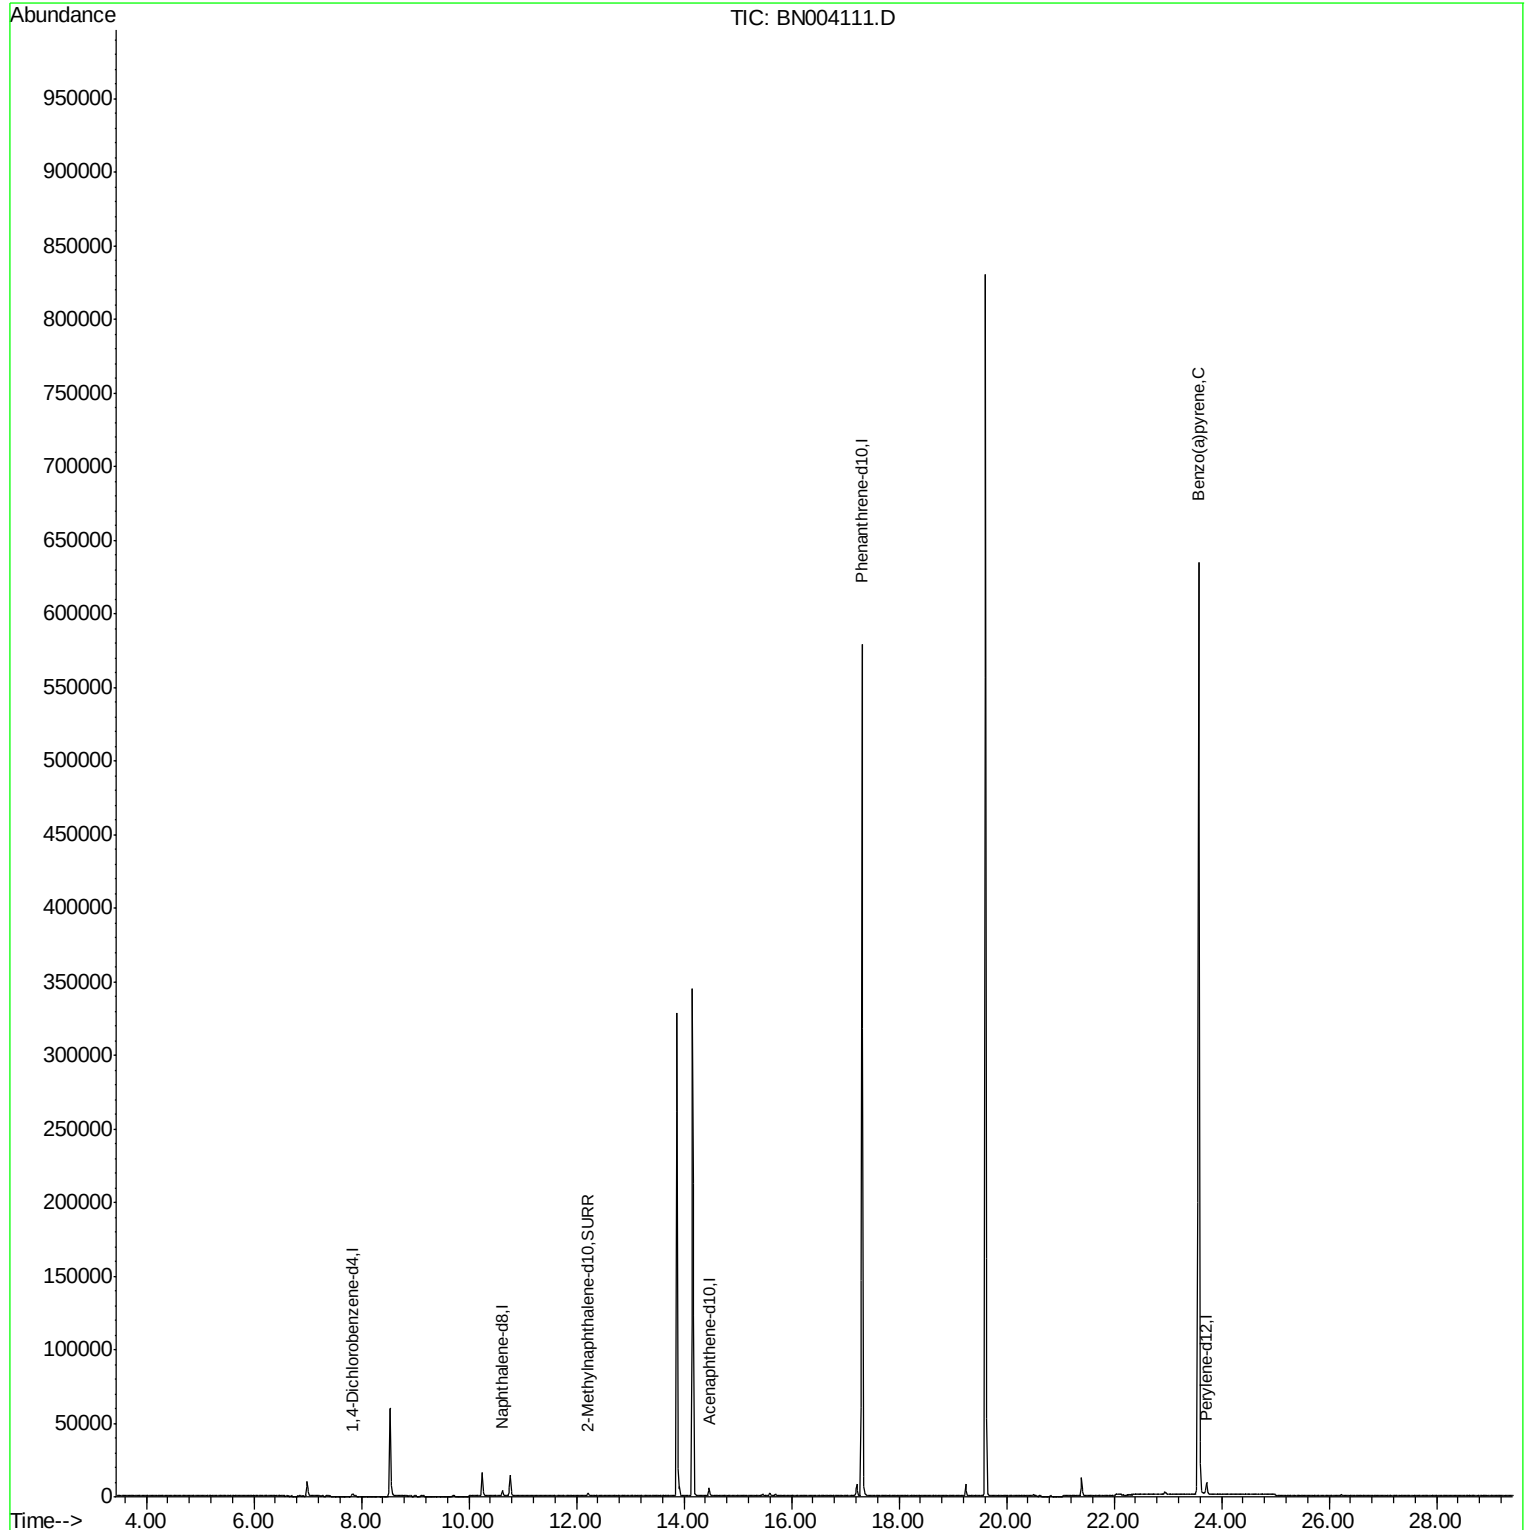

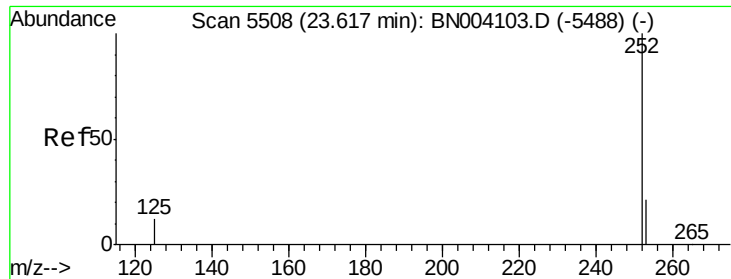

#23

Benzo(a)pyrene

Concen: 0.072 ng/ul

RT: 23.57 min Scan# 5493

Delta R.T. -0.04 min

Lab File: BN004111.D


Acq: 19 Dec 2018 13:46

Instrument :

BNA_N

ClientSampleId :

F9E39

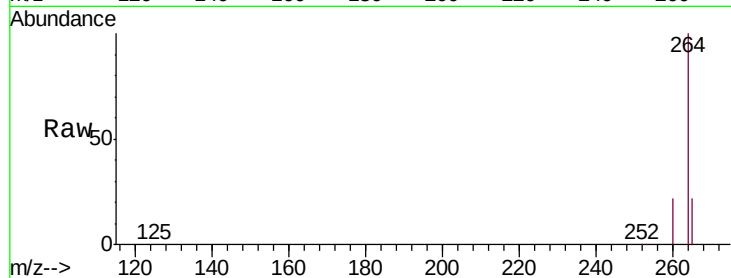

Tgt Ion:	252	Resp:	3141
Ion	Ratio	Lower	Upper
252	100		
253	37.0	19.0	28.4#
125	29.4	10.2	15.4#

