

Data File : BN004117.D
Acq On : 19 Dec 2018 17:17
Operator : JU/SJ
Sample : J6297-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E42

Quant Time: Dec 20 05:52:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 05:49:27 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	1325	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	6964	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	4481	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	761792	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.72	264	12333	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	3051	0.29	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.46	166	1188	0.058	ng/ul#	15
23) Benzo(a)pyrene	23.58	252	3040	0.069	ng/ul#	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN004117.D
Acq On : 19 Dec 2018 17:17
Operator : JU/SJ
Sample : J6297-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E42

Quant Time: Dec 20 05:52:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 05:49:27 2018
Response via : Initial Calibration




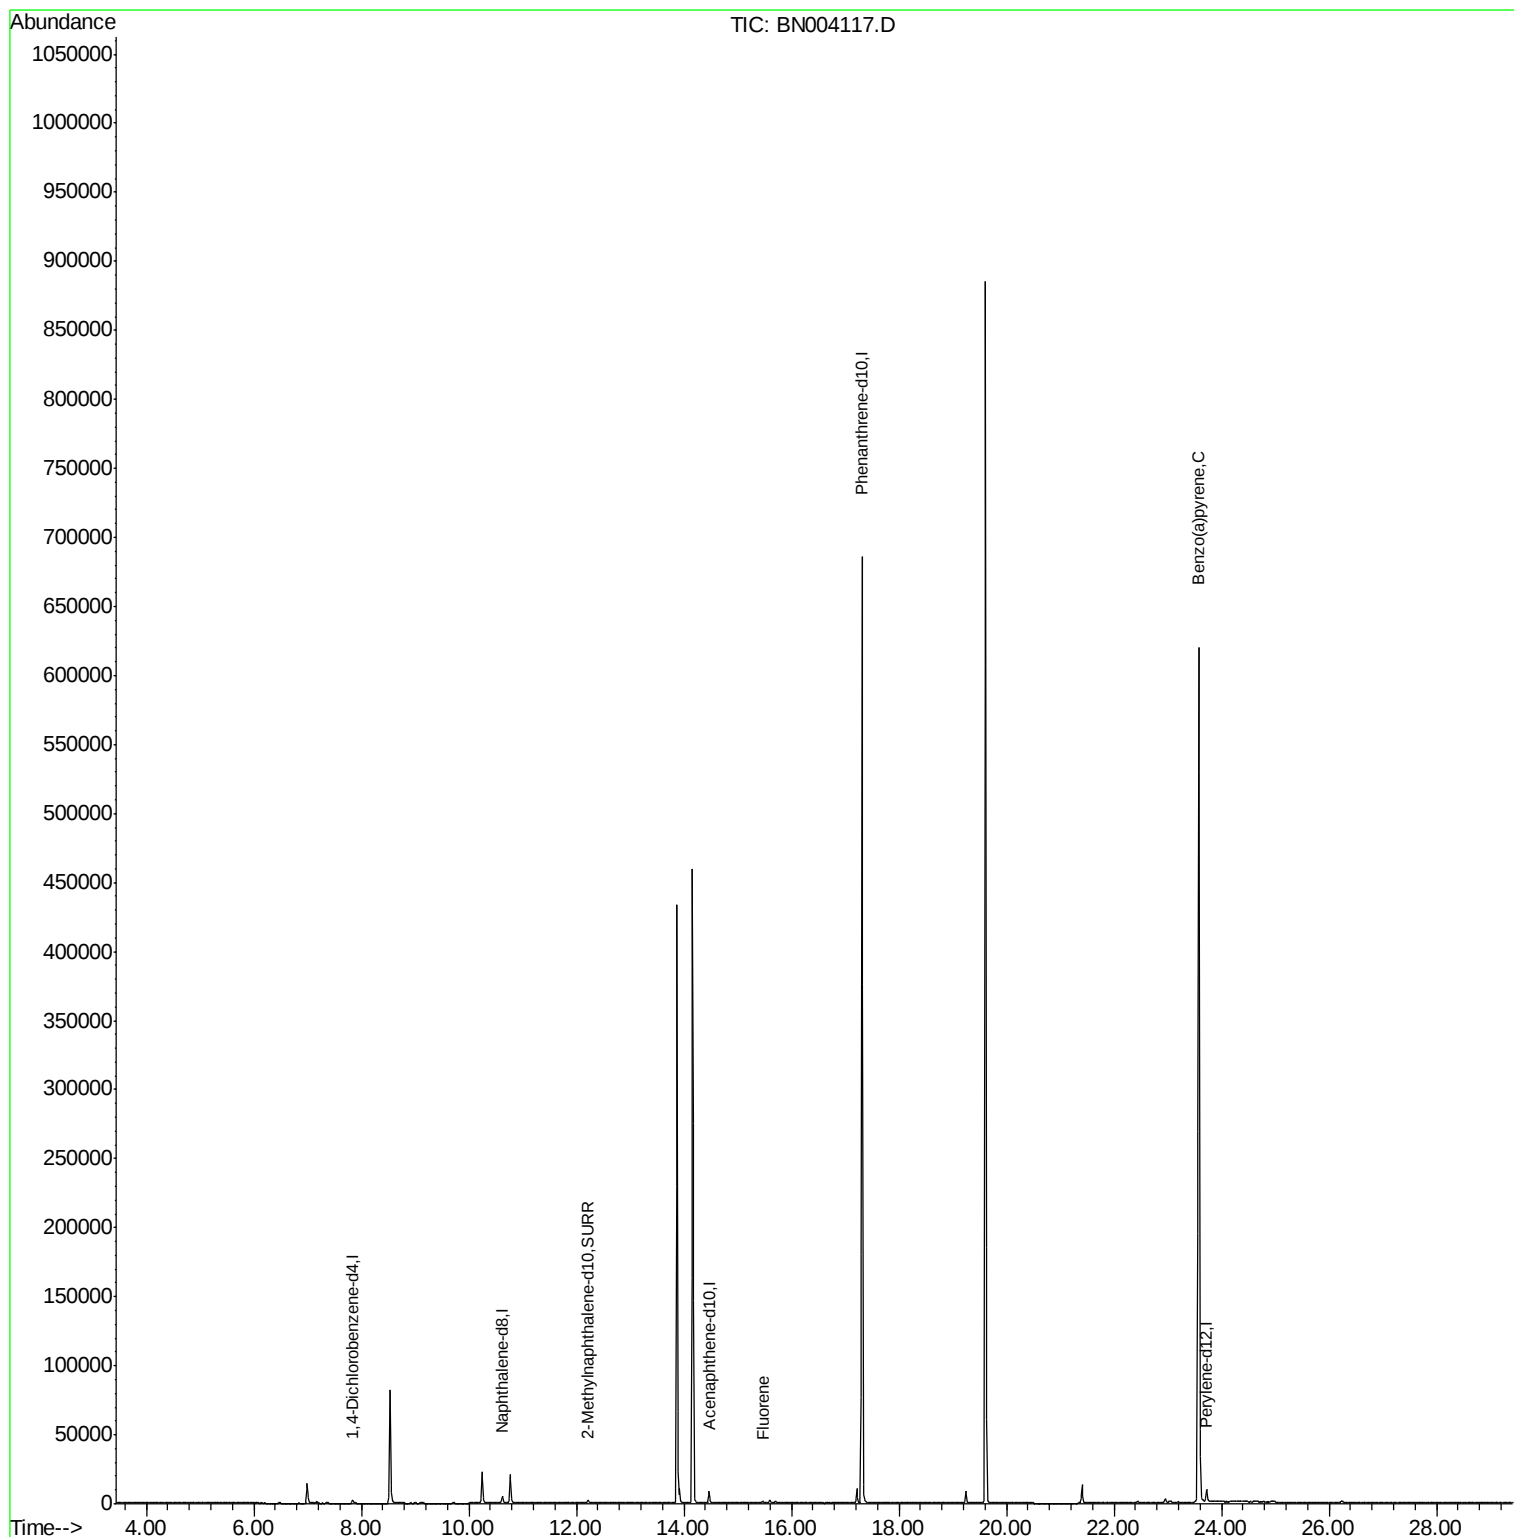


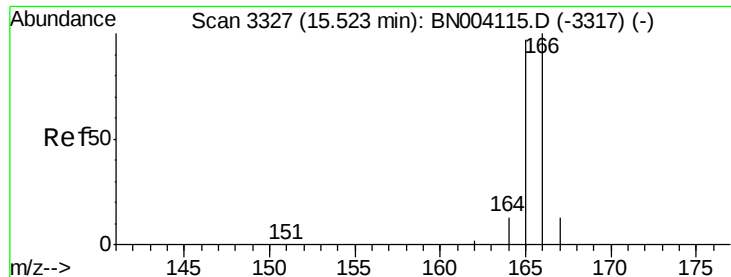

#9
Fluorene
 Concen: 0.058 ng/ul
 RT: 15.46 min Scan# 3314
 Delta R.T. -0.06 min
 Lab File: BN004117.D
 Acq: 19 Dec 2018 17:17

Instrument :
 BNA_N
 ClientSampleId :
 F9E42

Tgt Ion:166 Resp: 1188
 Ion Ratio Lower Upper
 166 100
 165 10.3 78.3 117.5#
 167 38.6 11.3 16.9#

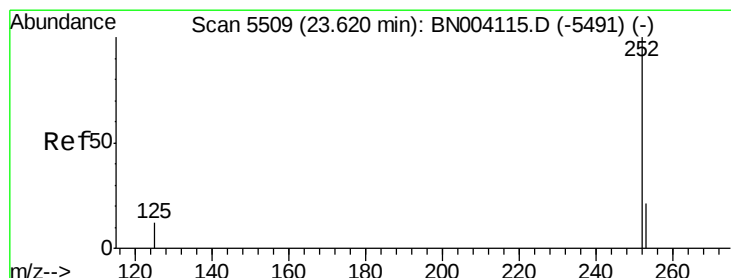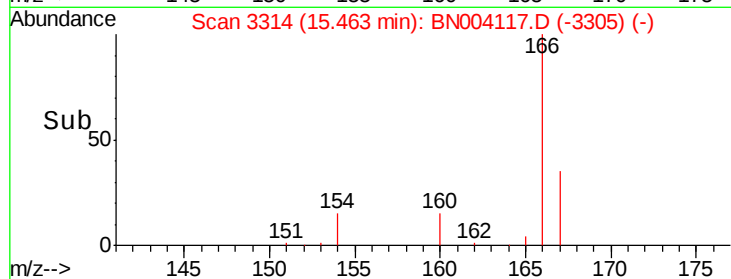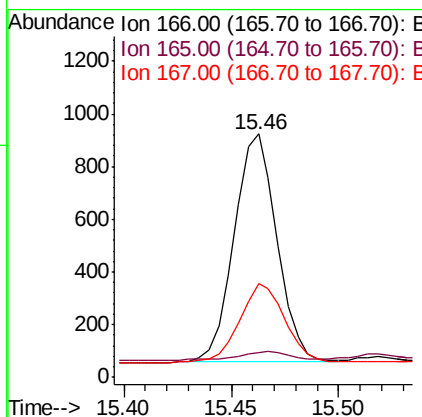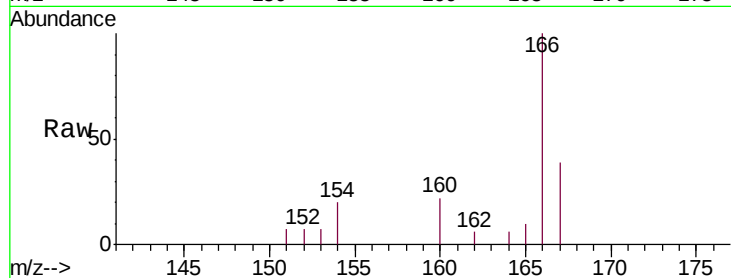

#23
Benzo(a)pyrene
 Concen: 0.069 ng/ul
 RT: 23.58 min Scan# 5495
 Delta R.T. -0.04 min
 Lab File: BN004117.D
 Acq: 19 Dec 2018 17:17

Tgt Ion:252 Resp: 3040
 Ion Ratio Lower Upper
 252 100
 253 37.8 19.0 28.4#
 125 29.1 10.2 15.4#

