

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (QT Reviewed)


Data File : BN004134.D
Acq On : 20 Dec 2018 03:15
Operator : JU/SJ
Sample : J6299-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F24

Manual Integrations
APPROVED

Sohil
12/20/2018 2:03:54 PM

Quant Time: Dec 20 07:32:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

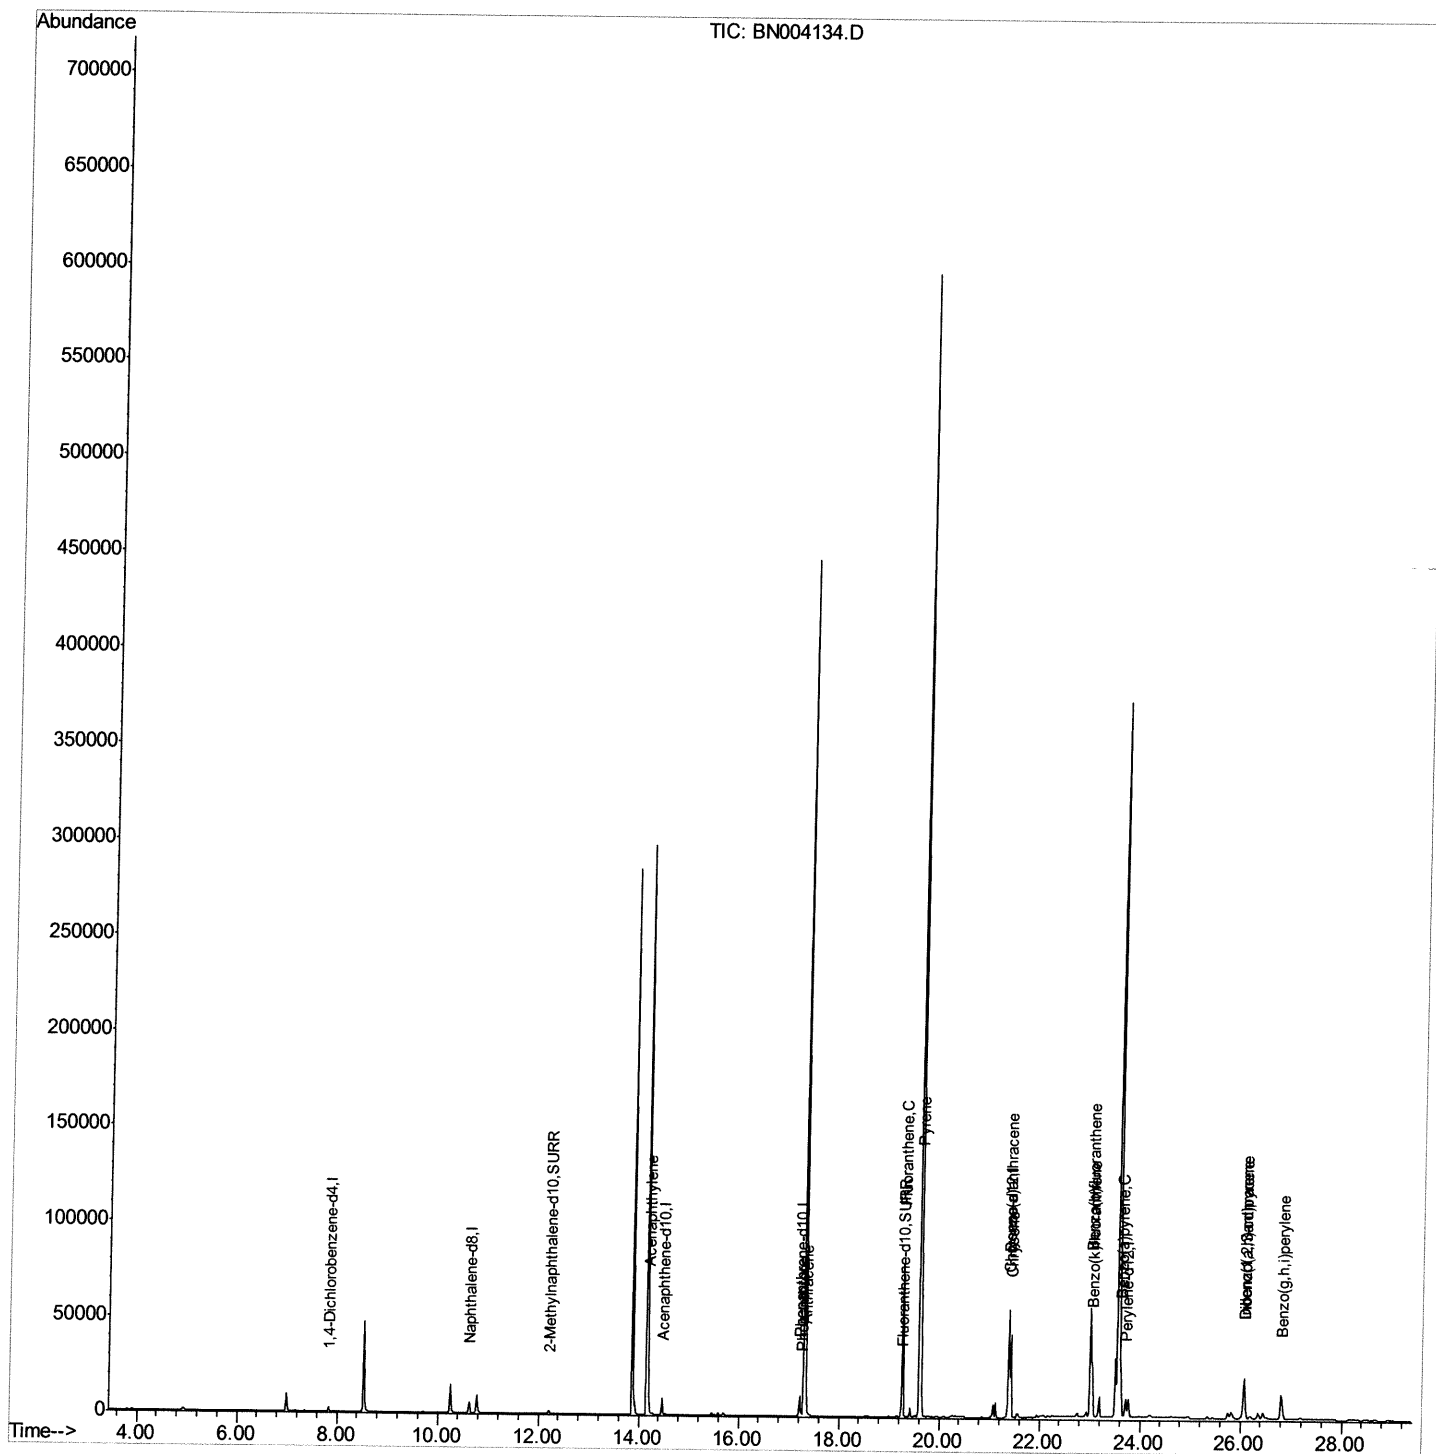

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Qedit)




Data File : BN004134.D
Acq On : 20 Dec 2018 03:15
Operator : JU/SJ
Sample : J6299-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F24

Manual Integrations
APPROVED

Sohil
12/20/2018 2:03:54 PM

Quant Time: Dec 20 07:20:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

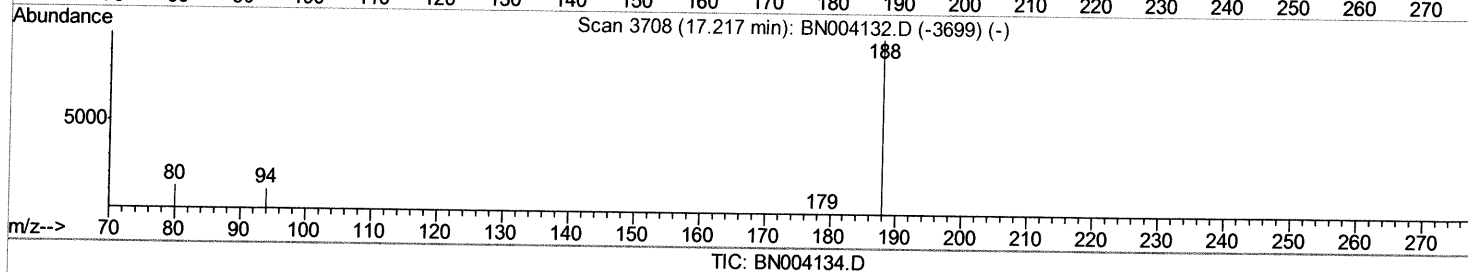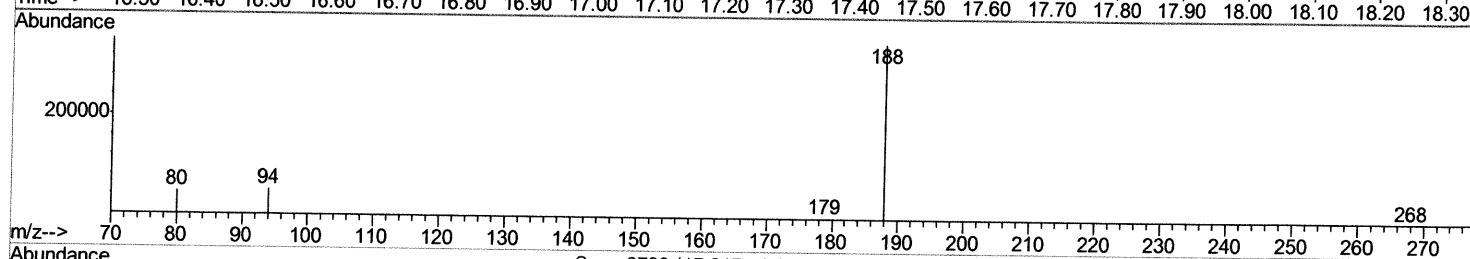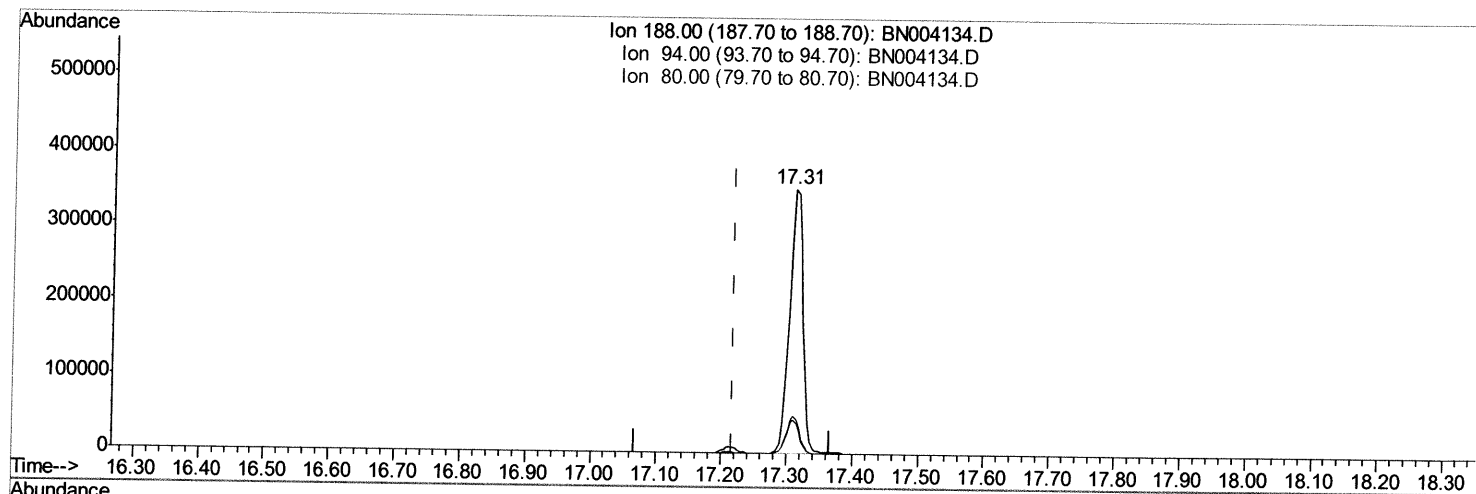

(10) Phenanthrene-d10 (I)

17.310min (+0.093) 0.40ng/ul

response 488821

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	14.18#
80.00	11.60	12.87
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Qedit)


Data File : BN004134.D
Acq On : 20 Dec 2018 03:15
Operator : JU/SJ
Sample : J6299-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F24

Manual Integrations
APPROVED

Sohil
12/20/2018 2:03:54 PM

Quant Time: Dec 20 07:20:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

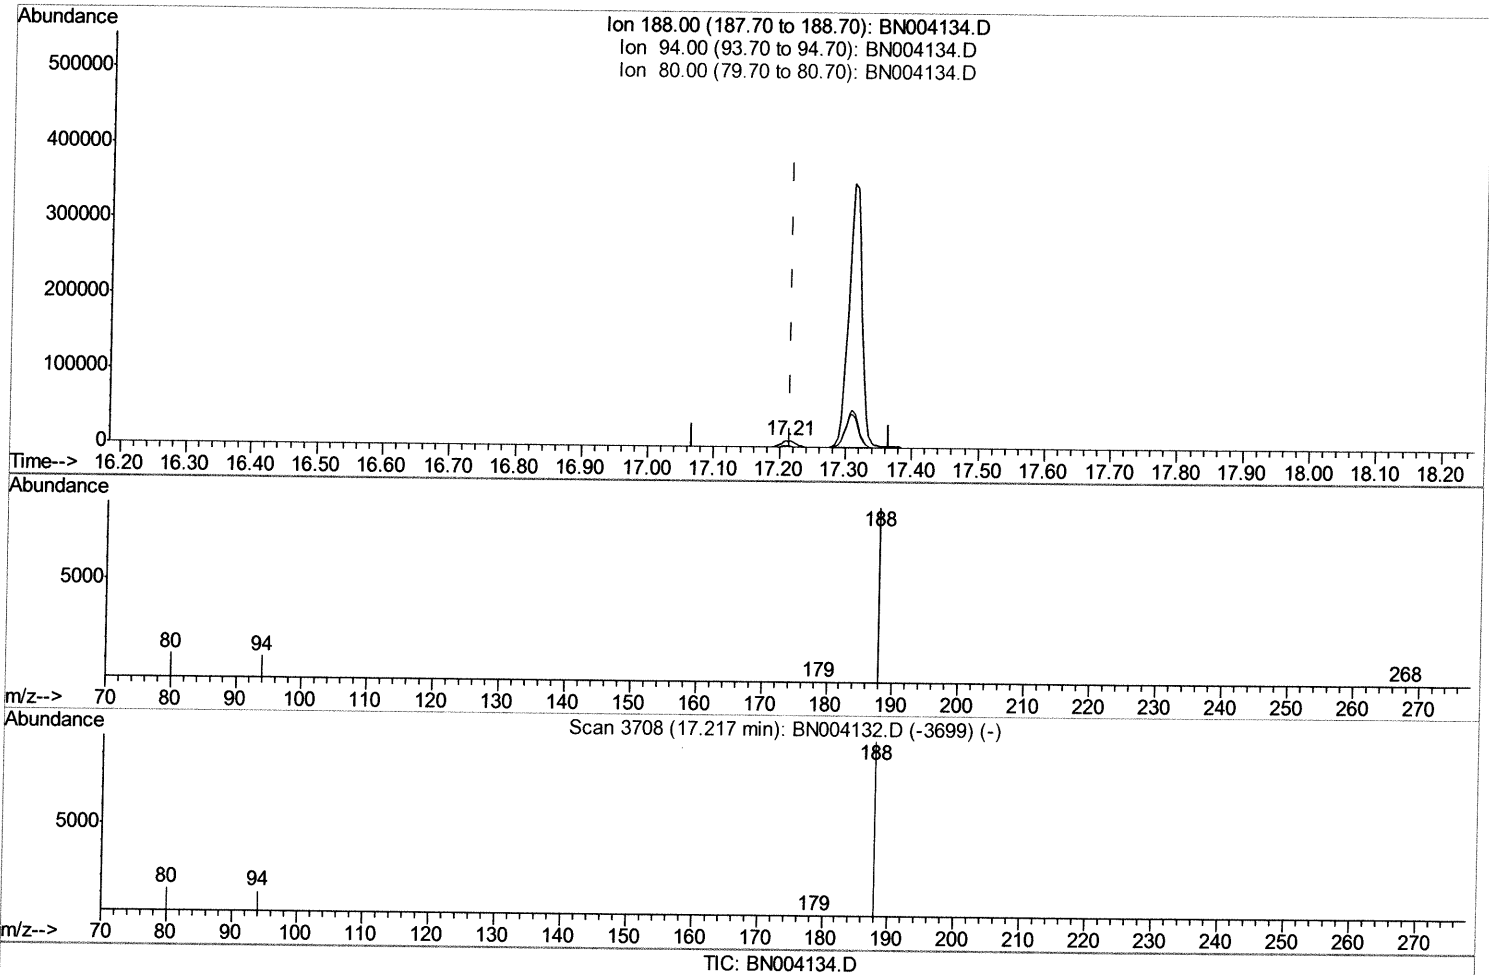

(10) Phenanthrene-d10 (I)

17.213min (-0.004) 0.40ng/ul m

response 12457

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	12.56#
80.00	11.60	13.86
0.00	0.00	0.00

> SJ
12/20/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Qedit)


Data File : BN004134.D
Acq On : 20 Dec 2018 03:15
Operator : JU/SJ
Sample : J6299-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F24

Manual Integrations
APPROVED

Sohil
12/20/2018 2:03:54 PM

Quant Time: Dec 20 07:28:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

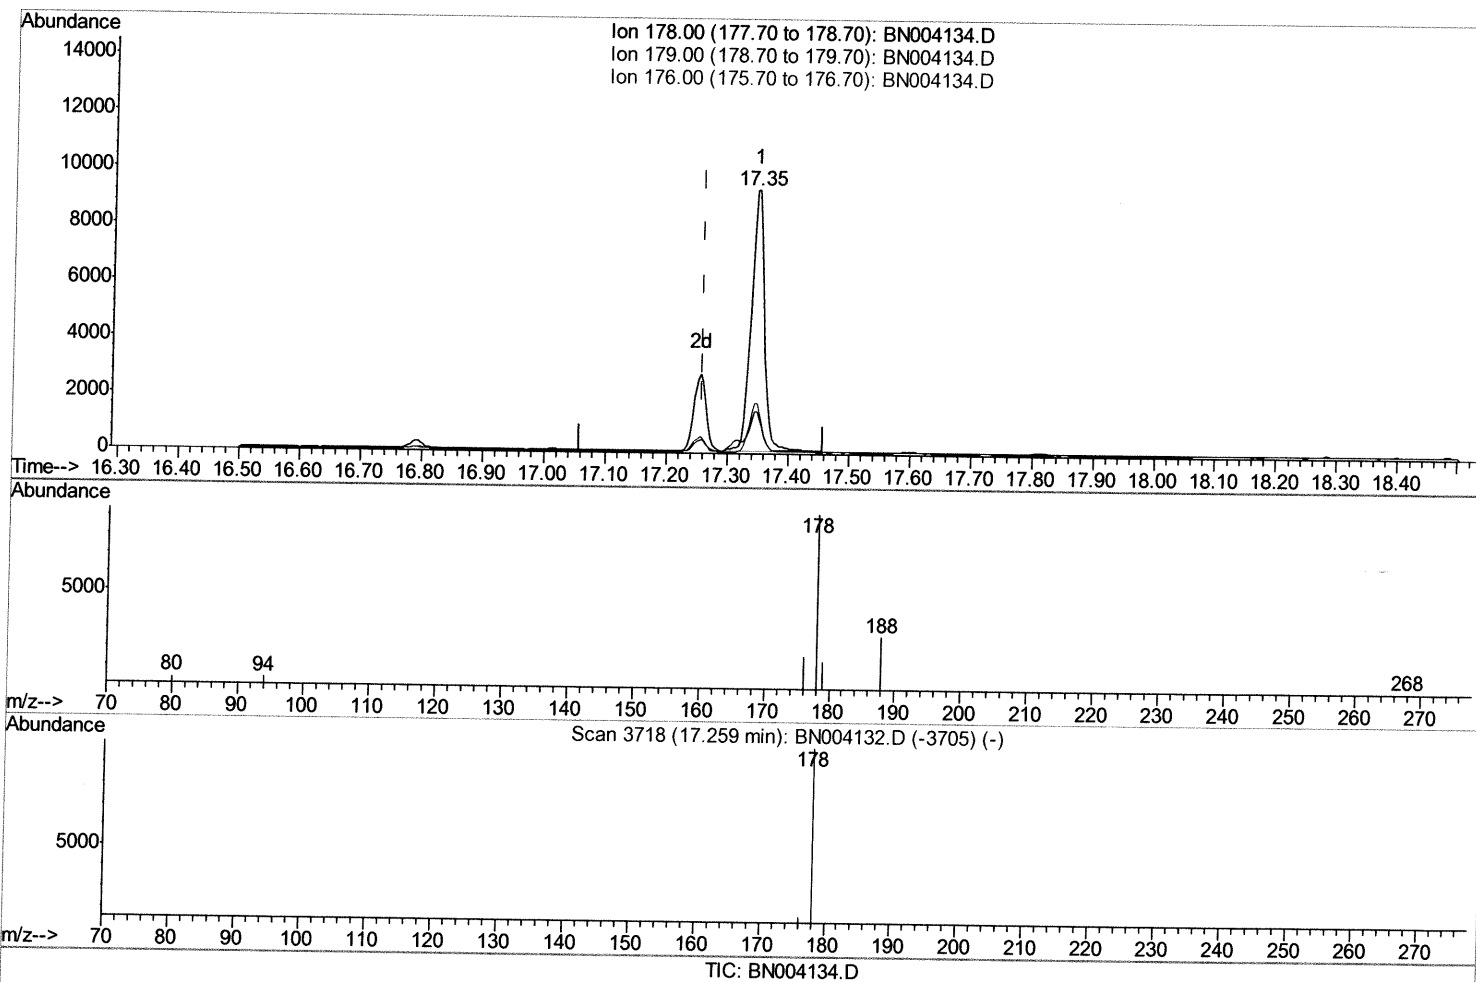

(12) Phenanthrene

17.348min (+0.089) 0.36ng/ul

response 14696

Ion	Exp%	Act%
178.00	100	100
179.00	15.60	16.04
176.00	18.70	18.92
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Qedit)




Data File : BN004134.D
Acq On : 20 Dec 2018 03:15
Operator : JU/SJ
Sample : J6299-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F24

Manual Integrations
APPROVED

Sohil
12/20/2018 2:03:54 PM

Quant Time: Dec 20 07:28:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

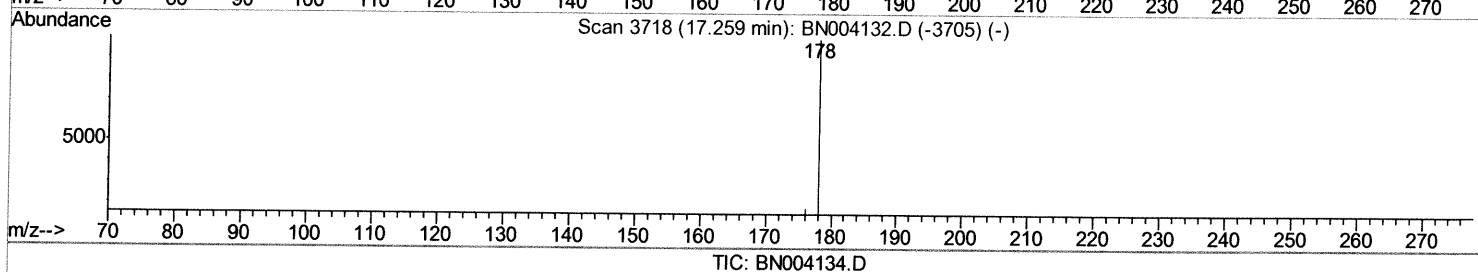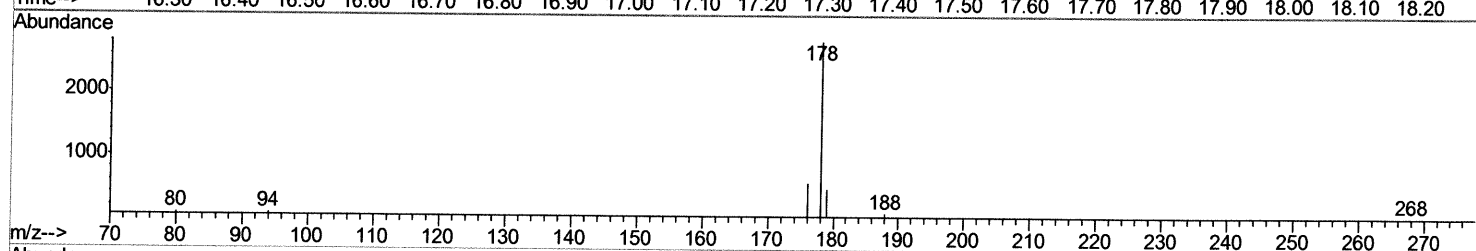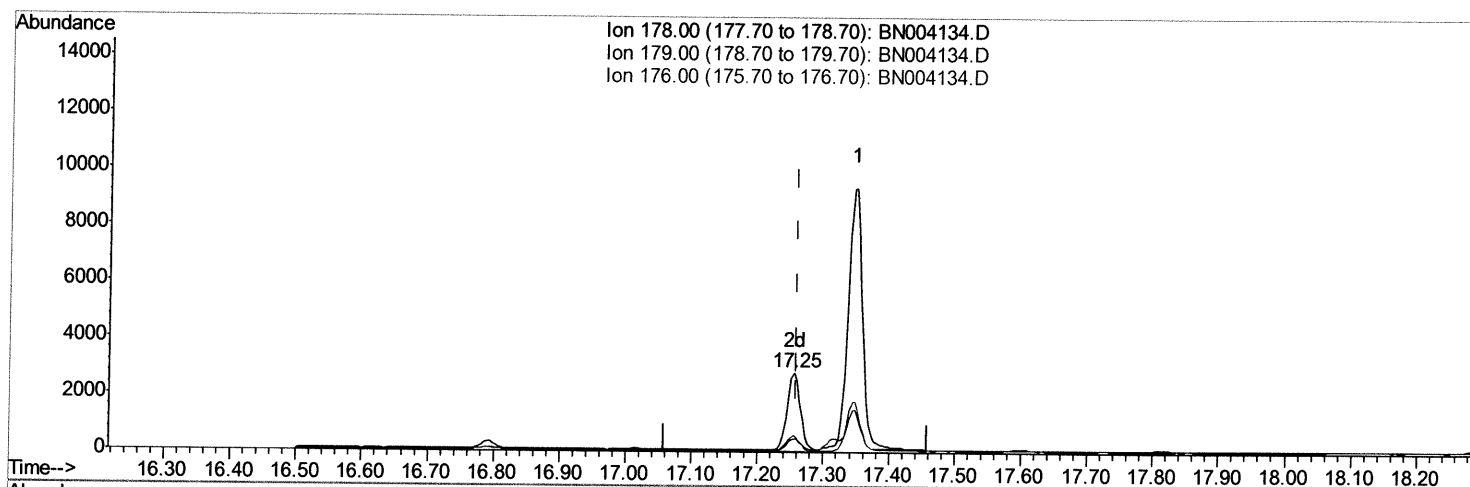

(12) Phenanthrene

17.255min (-0.004) 0.10ng/ul m

response 3927

Ion	Exp%	Act%
178.00	100	100
179.00	15.60	17.33
176.00	18.70	20.42
0.00	0.00	0.00

> 83
12/20/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Qedit)


Data File : BN004134.D
Acq On : 20 Dec 2018 03:15
Operator : JU/SJ
Sample : J6299-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F24

Manual Integrations
APPROVED

Sohil
12/20/2018 2:03:54 PM

Quant Time: Dec 20 07:28:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

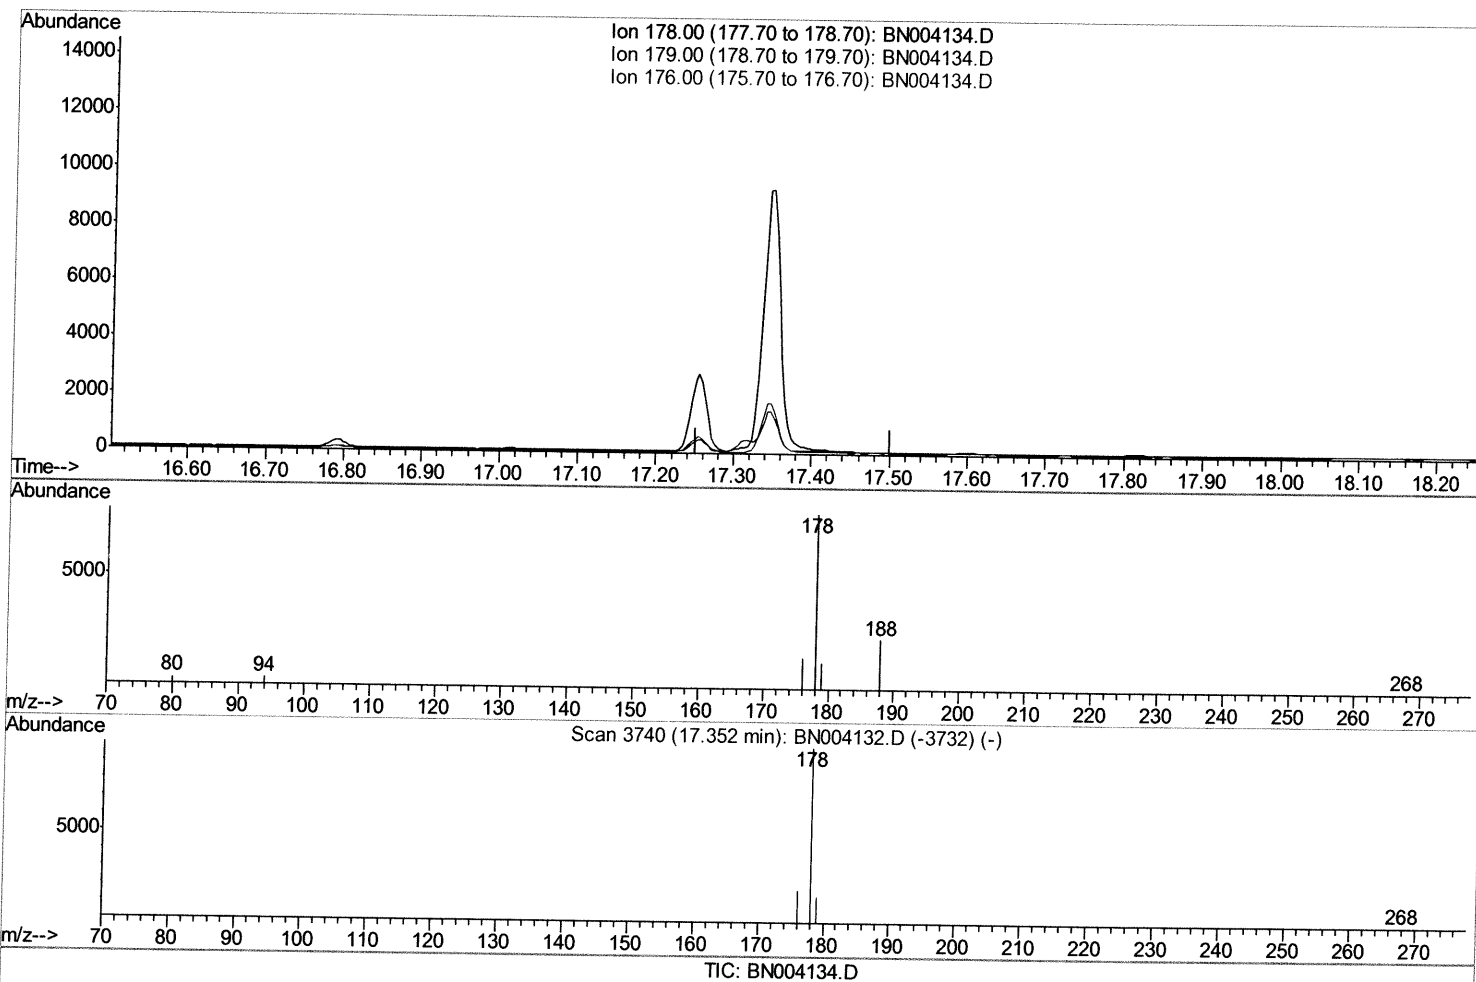

(13) Anthracene

17.352min (-17.352) 0.00ng/ul

response 0

Ion	Exp%	Act%
178.00	100	0.00
179.00	15.40	0.00#
176.00	18.50	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Qedit)




Data File : BN004134.D
Acq On : 20 Dec 2018 03:15
Operator : JU/SJ
Sample : J6299-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F24

Manual Integrations
APPROVED

Sohil
12/20/2018 2:03:54 PM

Quant Time: Dec 20 07:28:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

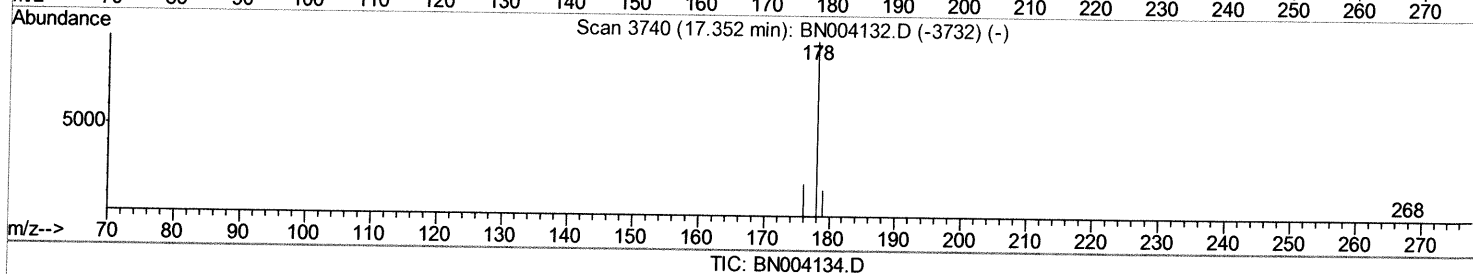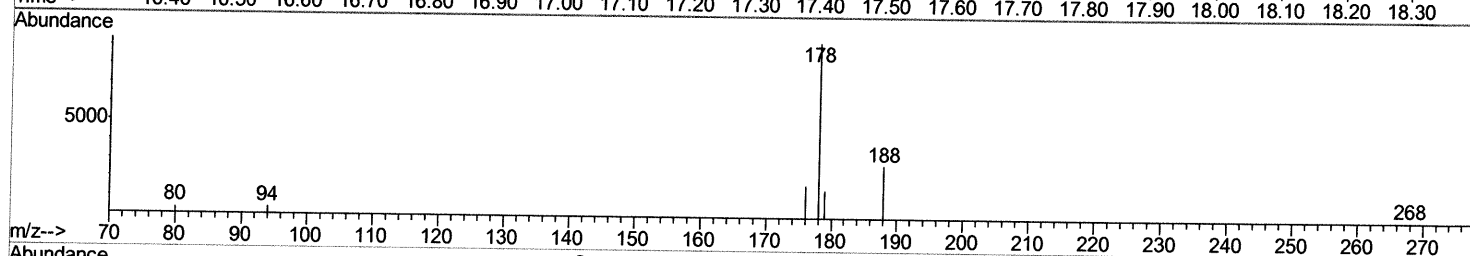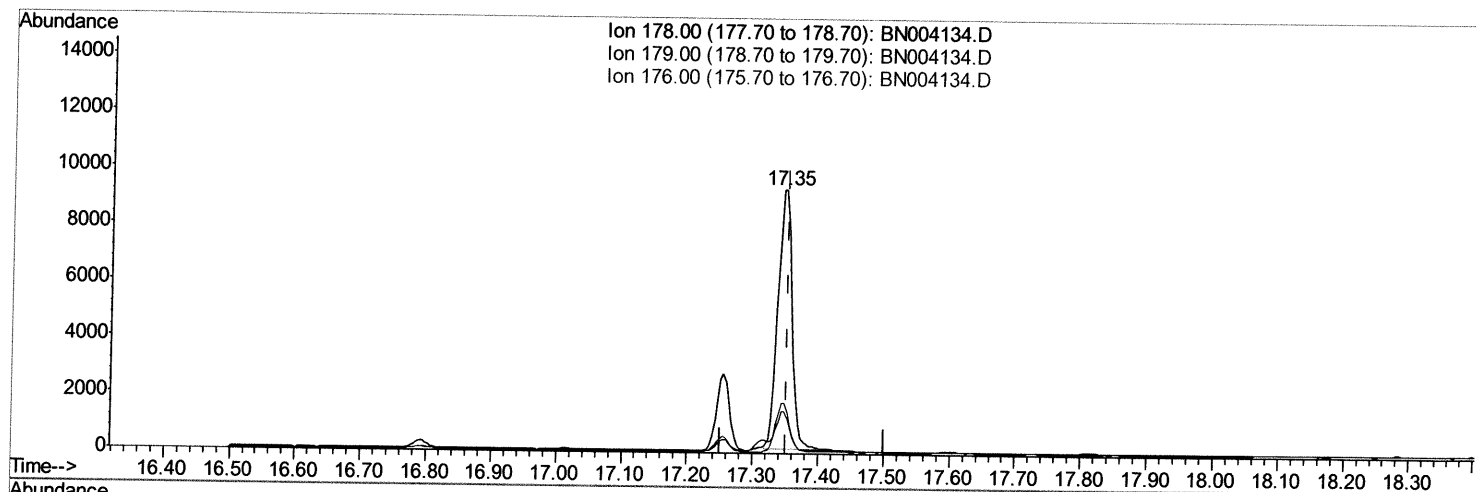

(13) Anthracene

17.348min (-0.004) 0.41ng/ul m

> SJ
12/20/18

response 13761

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	16.04
176.00	18.50	18.92
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Qedit)




Data File : BN004134.D
Acq On : 20 Dec 2018 03:15
Operator : JU/SJ
Sample : J6299-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F24

Manual Integrations
APPROVED

Sohil
12/20/2018 2:03:54 PM

Quant Time: Dec 20 07:28:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

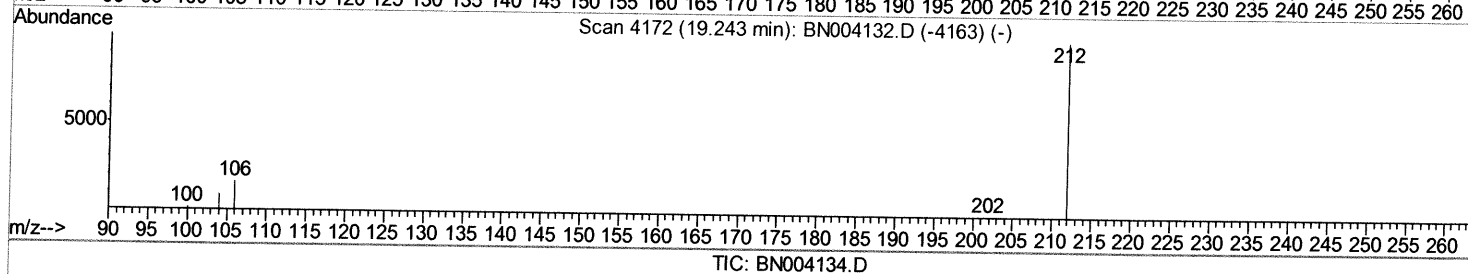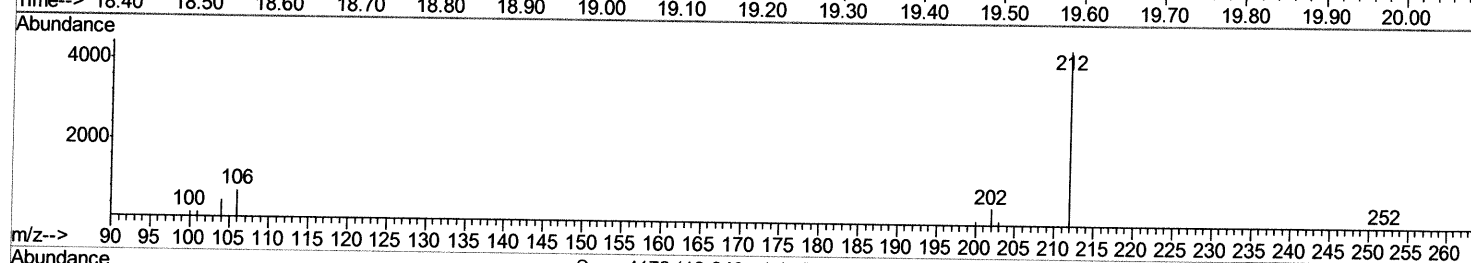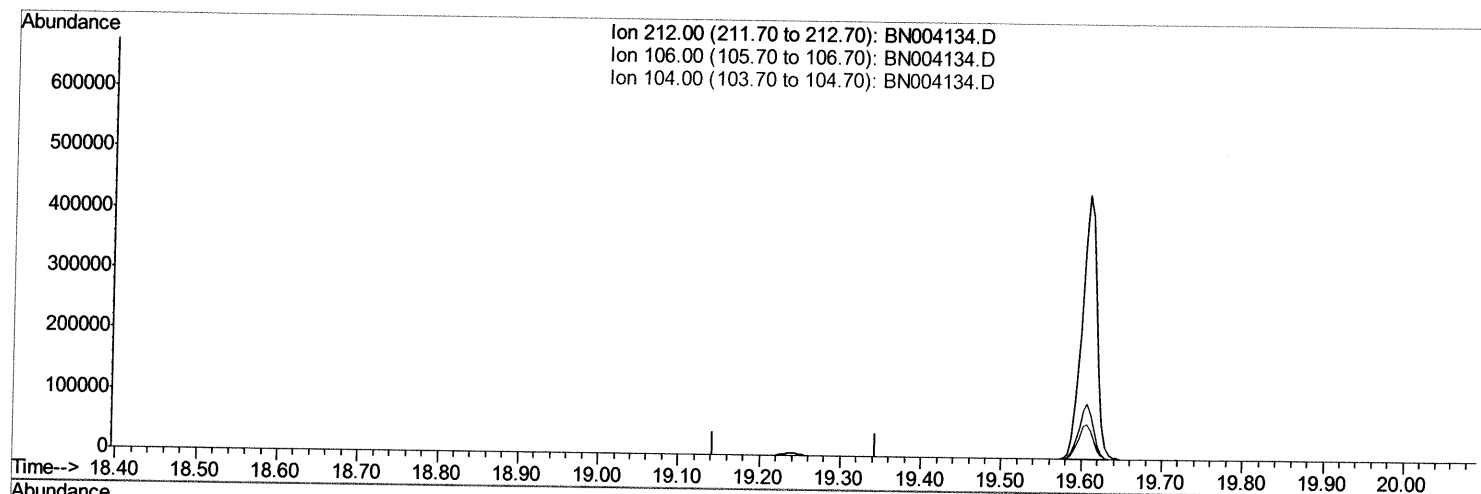

(14) Fluoranthene-d10 (SURR)

19.243min (-19.243) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Qedit)




Data File : BN004134.D
Acq On : 20 Dec 2018 03:15
Operator : JU/SJ
Sample : J6299-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F24

Manual Integrations
APPROVED

Sohil
12/20/2018 2:03:54 PM

Quant Time: Dec 20 07:28:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

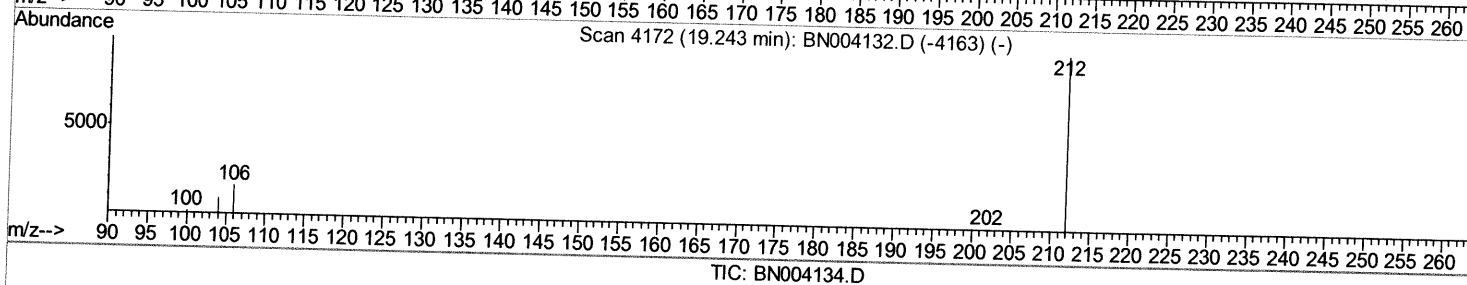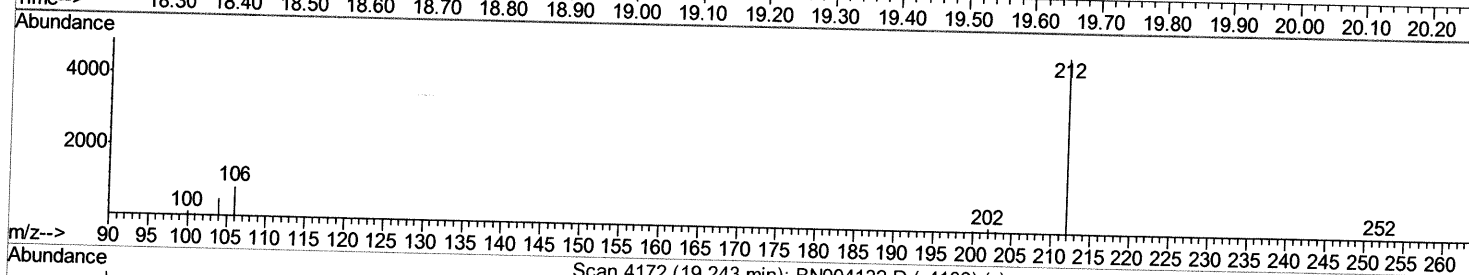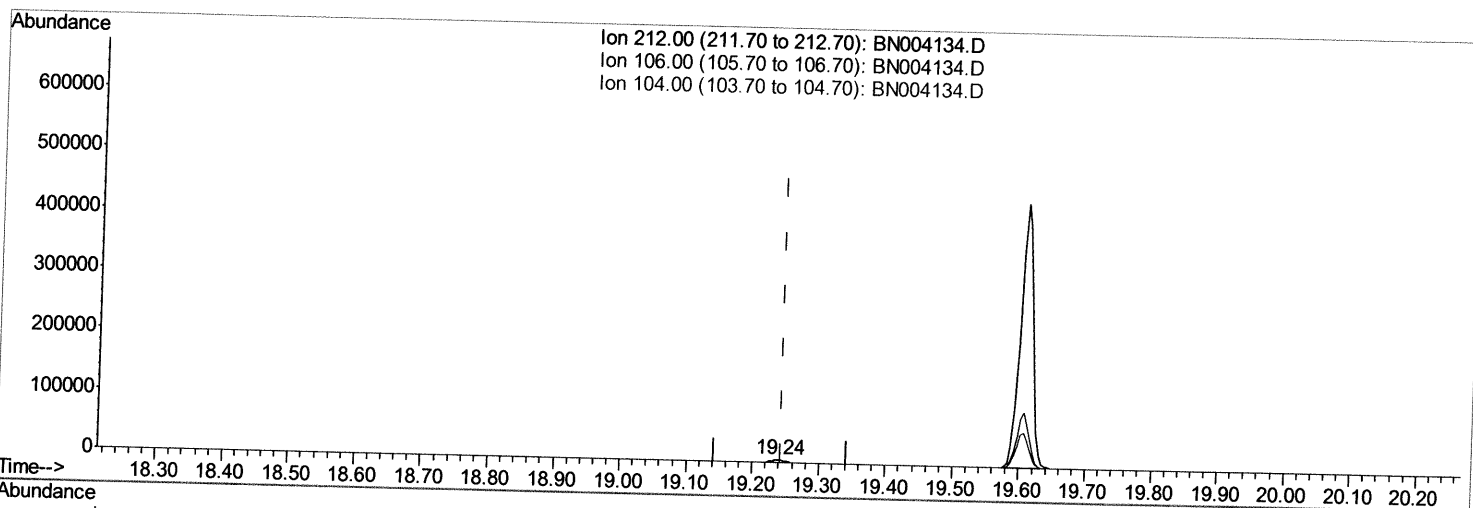

(14) Fluoranthene-d10 (SURR)

19.239min (-0.005) 0.18ng/ul m

response 6562

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

> SJ
12/20/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Qedit)


Data File : BN004134.D
Acq On : 20 Dec 2018 03:15
Operator : JU/SJ
Sample : J6299-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F24

Manual Integrations
APPROVED

Sohil
12/20/2018 2:03:54 PM

Quant Time: Dec 20 07:28:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

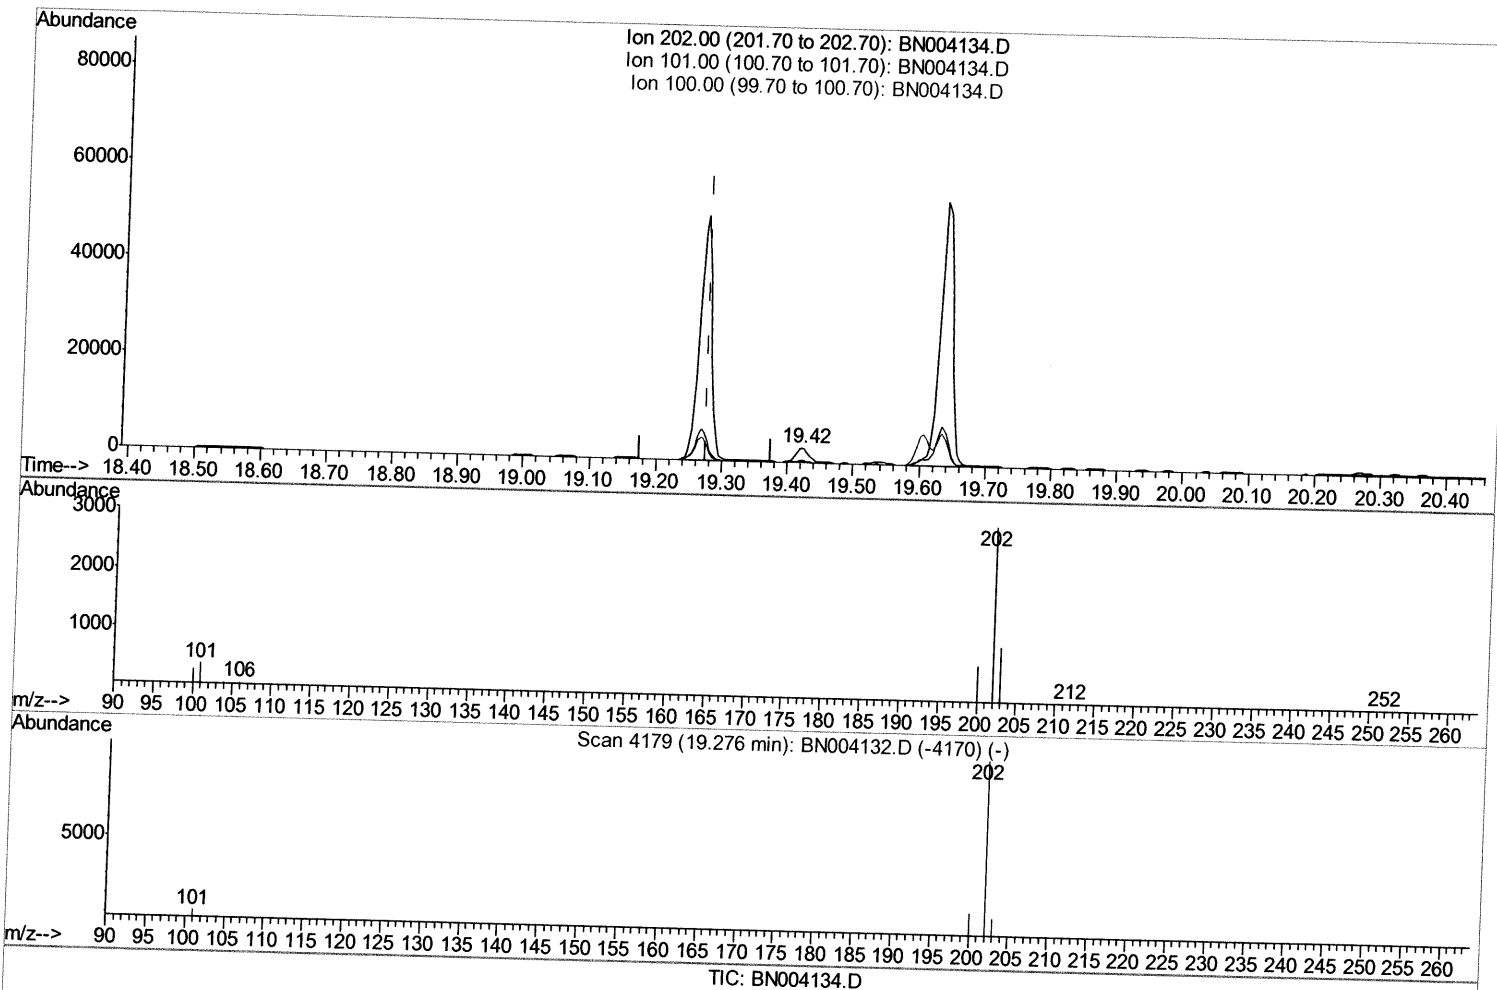

(15) Fluoranthene (C)

19.425min (+0.149) 0.08ng/ul

response 4003

Ion	Exp%	Act%
202.00	100	100
101.00	10.70	13.10
100.00	8.10	10.18
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Qedit)


Data File : BN004134.D
Acq On : 20 Dec 2018 03:15
Operator : JU/SJ
Sample : J6299-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F24

Manual Integrations
APPROVED

Sohil
12/20/2018 2:03:54 PM

Quant Time: Dec 20 07:28:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

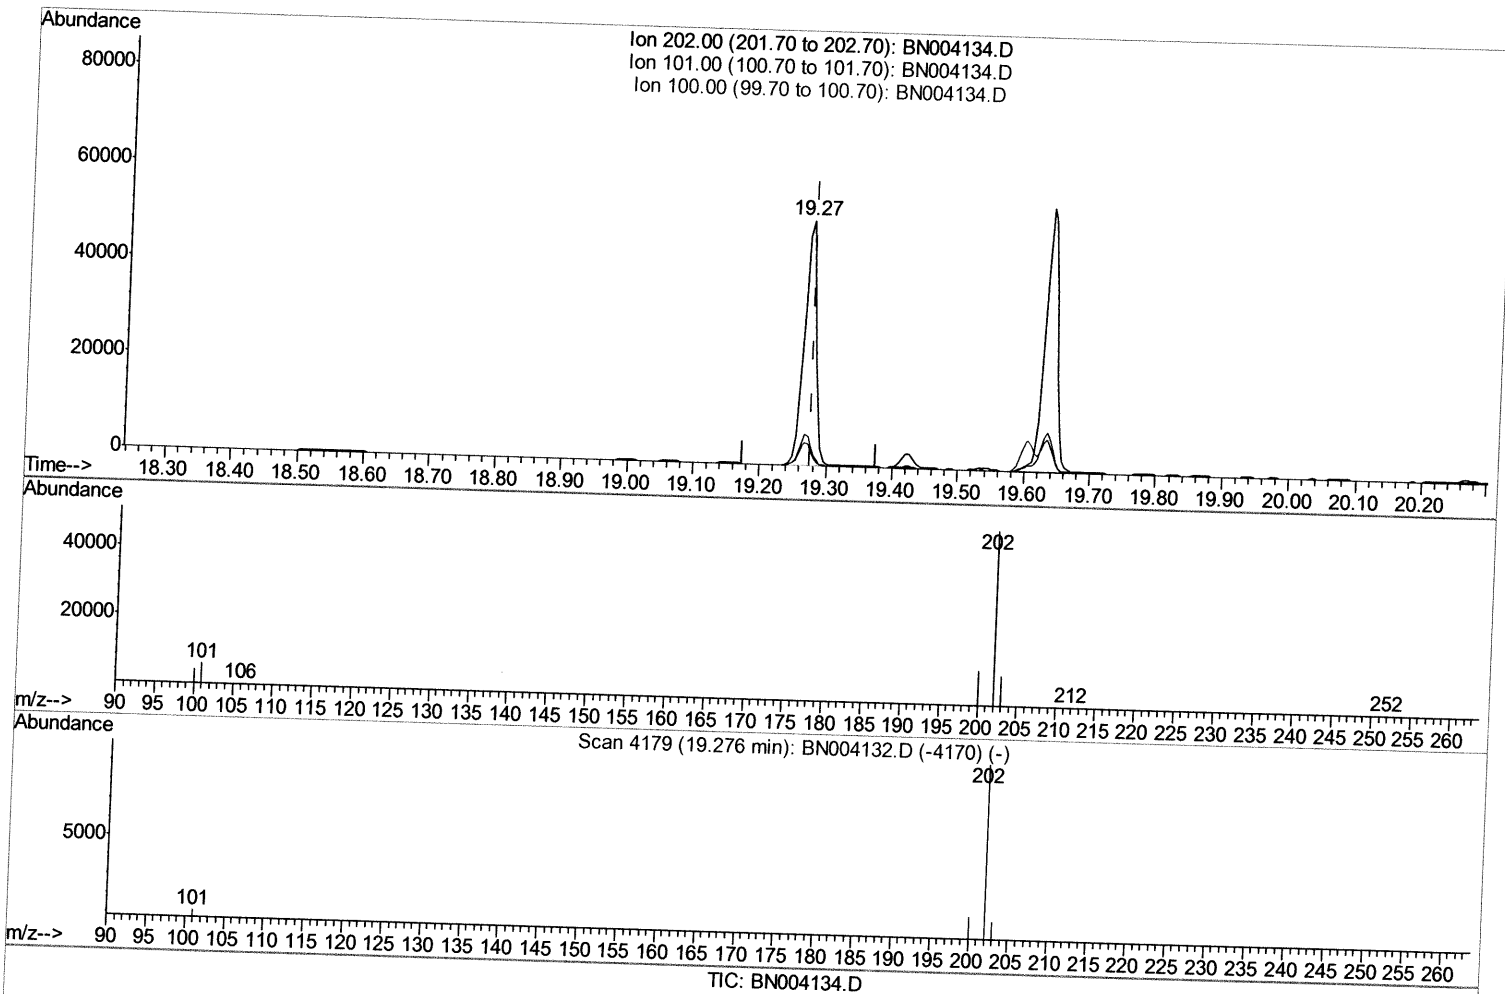

(15) Fluoranthene (C)

19.271min (-0.005) 1.34ng/ul m

> SJ
12/20/18

response 64591

Ion	Exp%	Act%
202.00	100	100
101.00	10.70	11.69
100.00	8.10	8.65
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Qedit)




Data File : BN004134.D
Acq On : 20 Dec 2018 03:15
Operator : JU/SJ
Sample : J6299-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9F24

Manual Integrations
APPROVED

Sohil
12/20/2018 2:03:54 PM

Quant Time: Dec 20 07:28:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

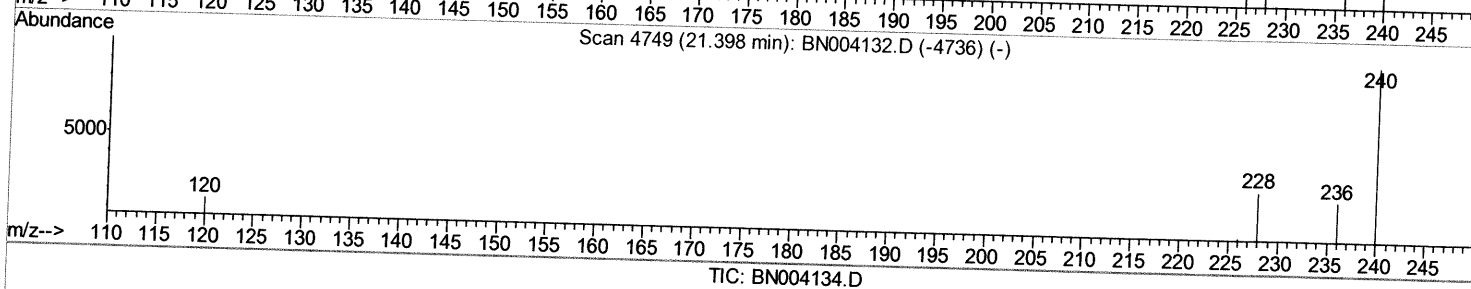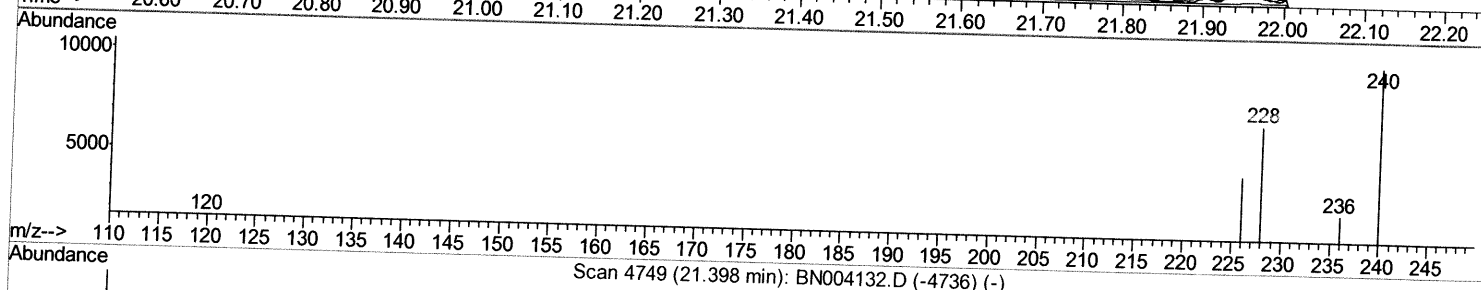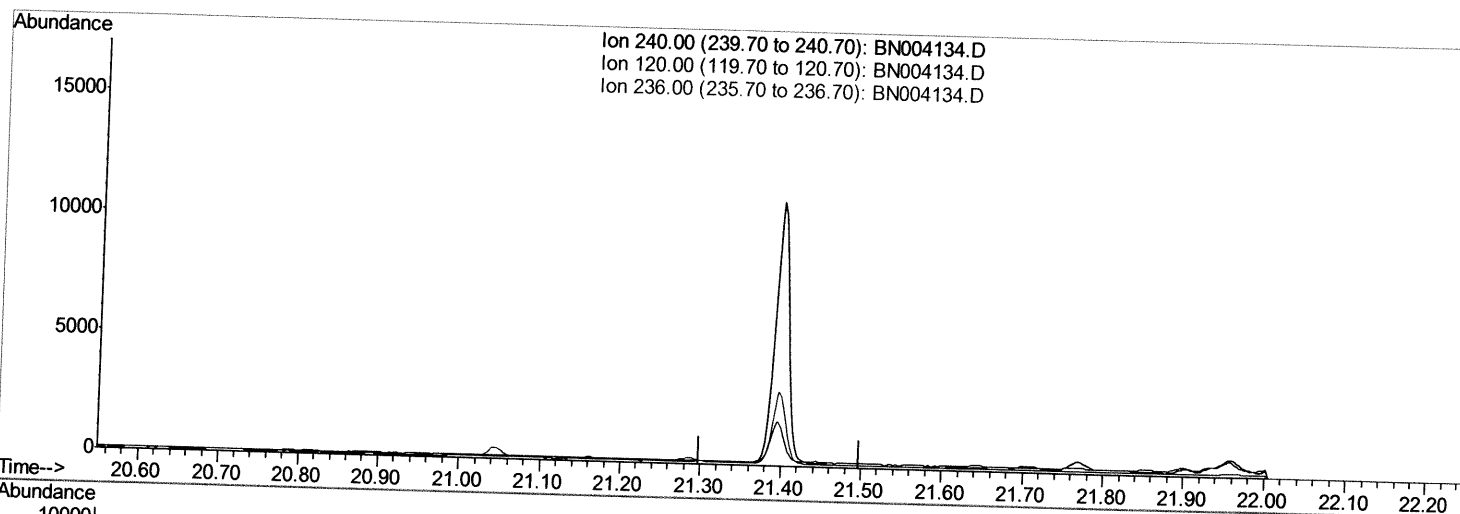

(16) Chrysene-d12 (I)

21.398min (-21.398) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Qedit)




Data File : BN004134.D
Acq On : 20 Dec 2018 03:15
Operator : JU/SJ
Sample : J6299-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9F24

Manual Integrations
APPROVED

Sohil
12/20/2018 2:03:54 PM

Quant Time: Dec 20 07:28:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

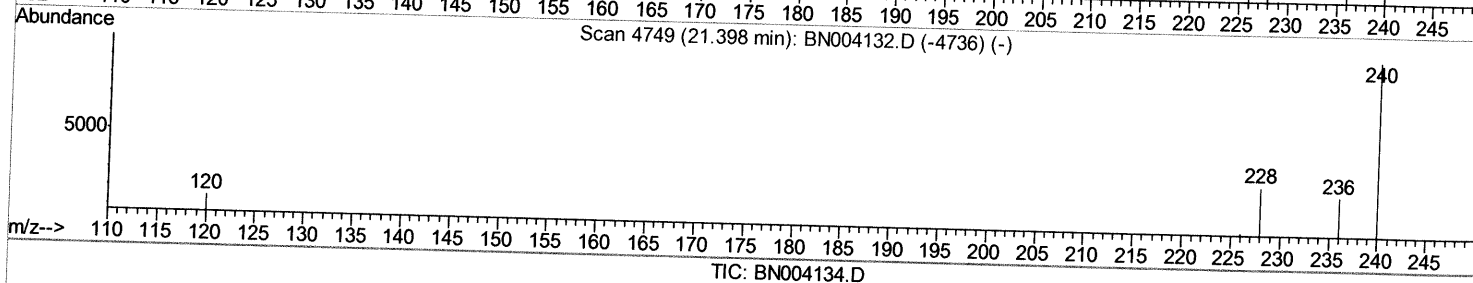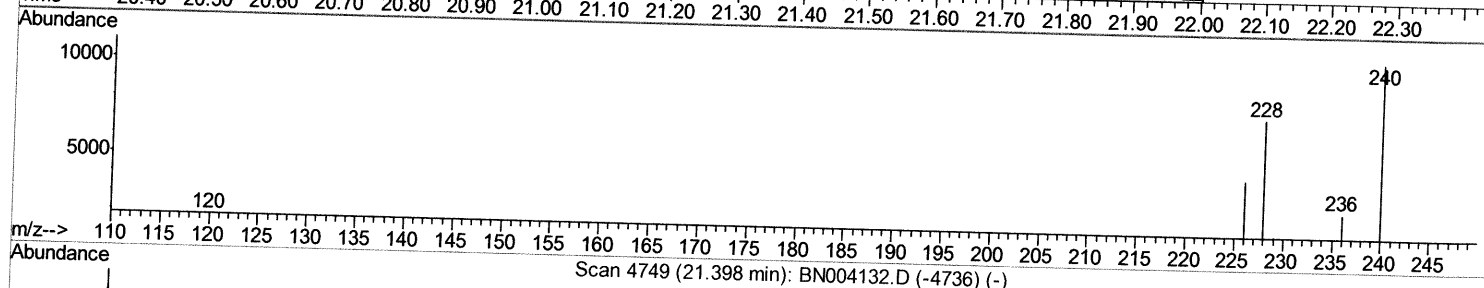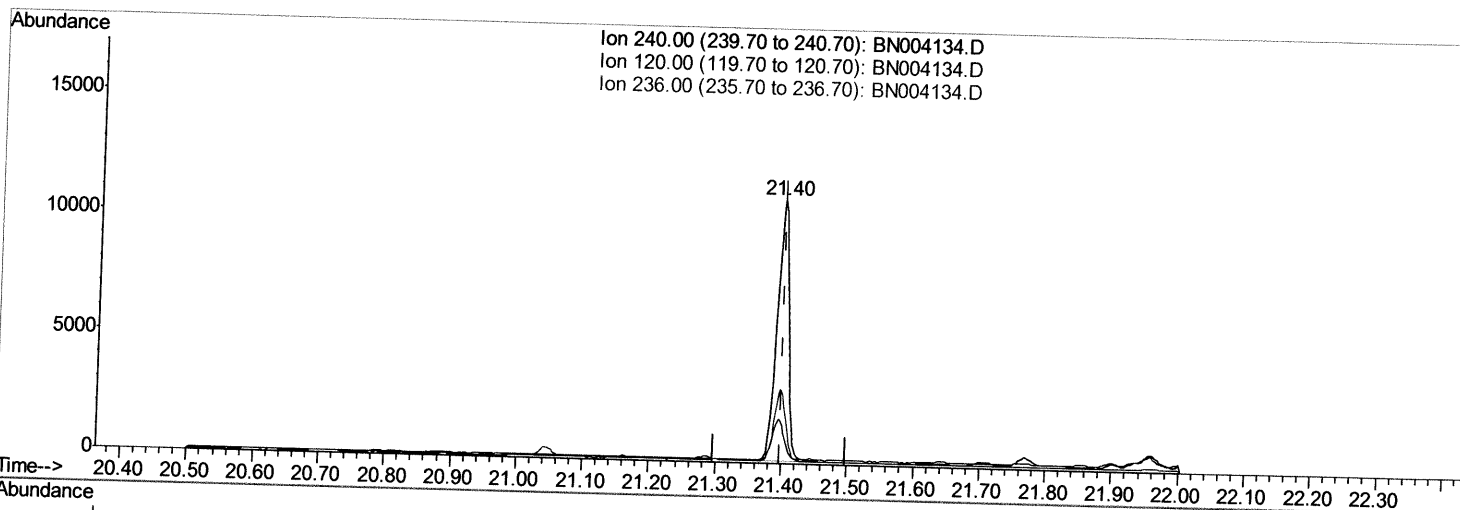

(16) Chrysene-d12 (I)

21.397min (-0.002) 0.40ng/ul m

response 13337

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	16.55
236.00	27.60	28.08
0.00	0.00	0.00

> SJ
12/20/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Qedit)


Data File : BN004134.D
Acq On : 20 Dec 2018 03:15
Operator : JU/SJ
Sample : J6299-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F24

Manual Integrations
APPROVED

Sohil
12/20/2018 2:03:54 PM

Quant Time: Dec 20 07:30:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

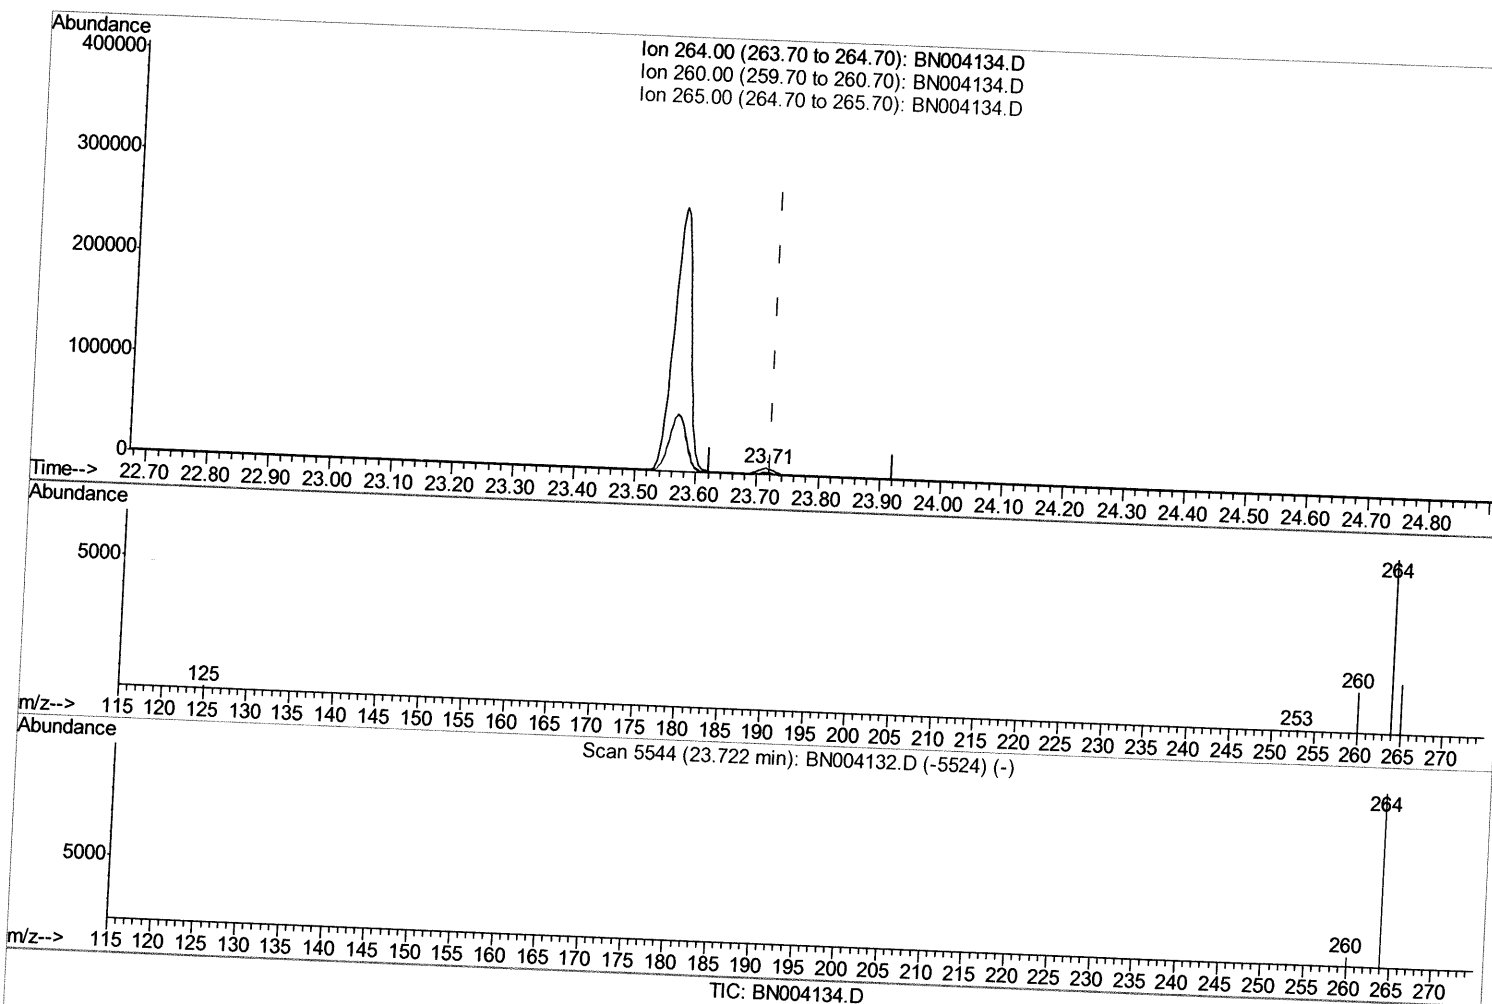

(20) Perylene-d12 (I)

23.715min (-0.007) 0.40ng/ul

response 13642

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	26.39
265.00	33.50	32.08
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Qedit)

Data File : BN004134.D
Acq On : 20 Dec 2018 03:15
Operator : JU/SJ
Sample : J6299-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F24

Manual Integrations
APPROVED
Sohil
12/20/2018 2:03:54 PM

Quant Time: Dec 20 07:30:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

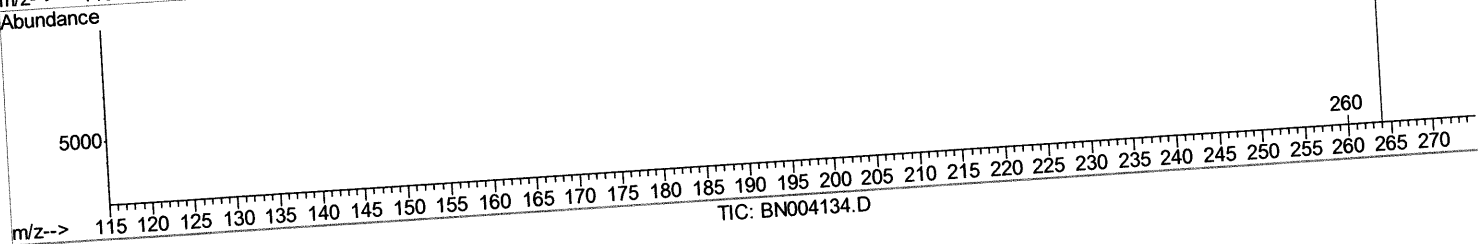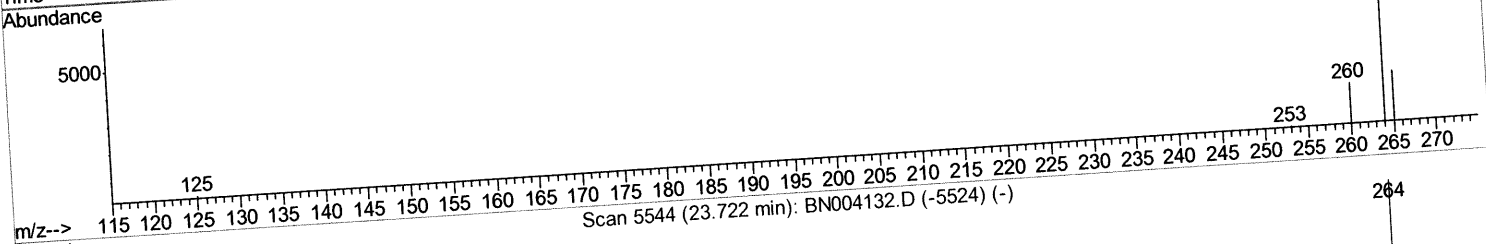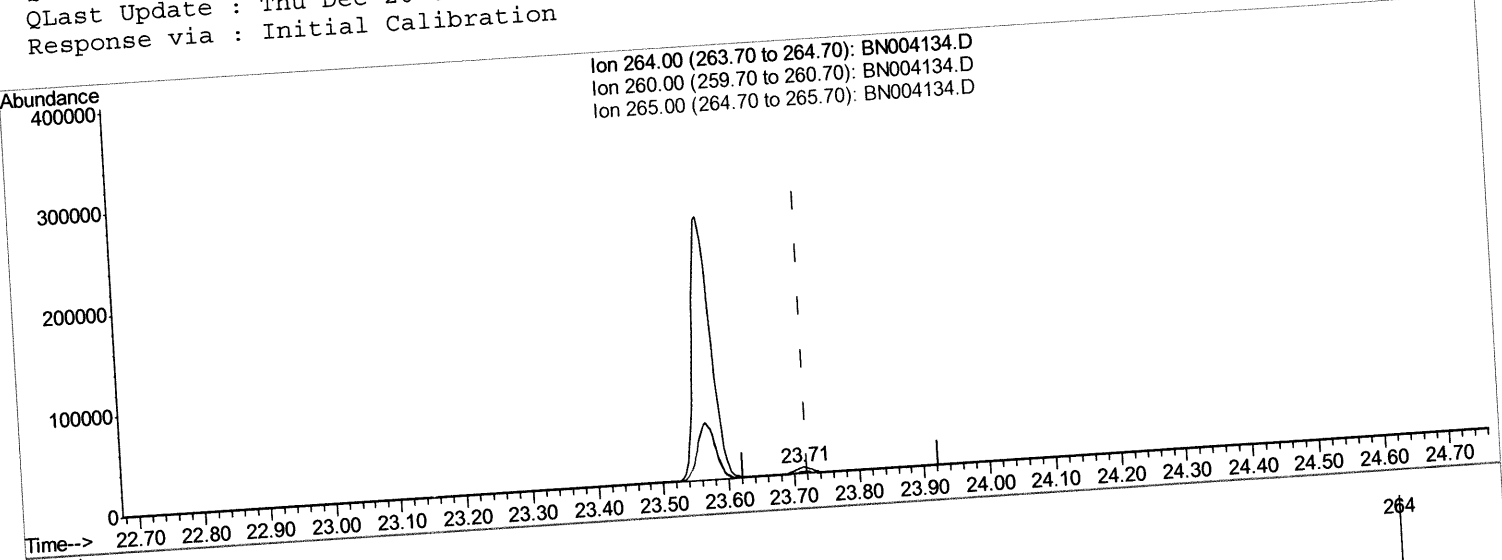

(20) Perylene-d12 (I)

23.715min (-0.007) 0.40ng/ul m

response 12411

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	26.39
265.00	33.50	32.08
0.00	0.00	0.00

JS
12/20/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Qedit)




Data File : BN004134.D
Acq On : 20 Dec 2018 03:15
Operator : JU/SJ
Sample : J6299-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F24

Manual Integrations
APPROVED

Sohil
12/20/2018 2:03:54 PM

Quant Time: Dec 20 07:31:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

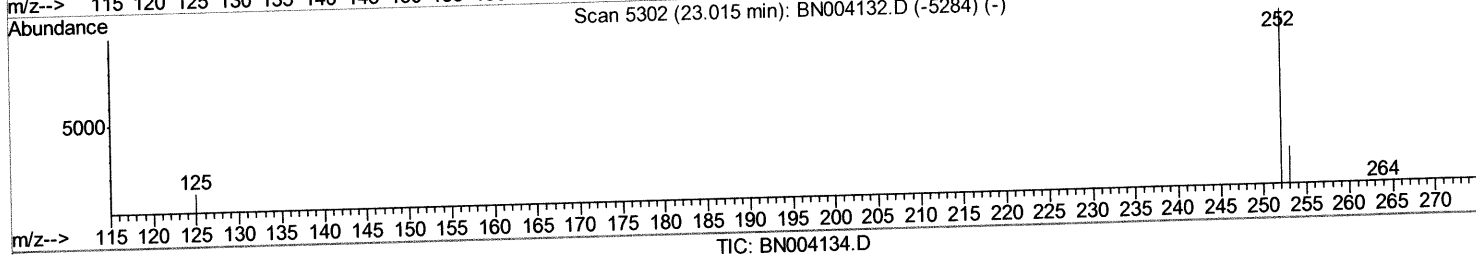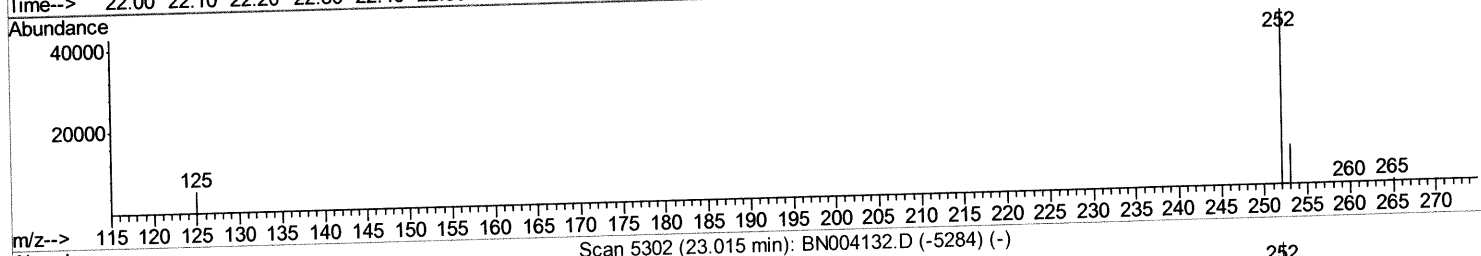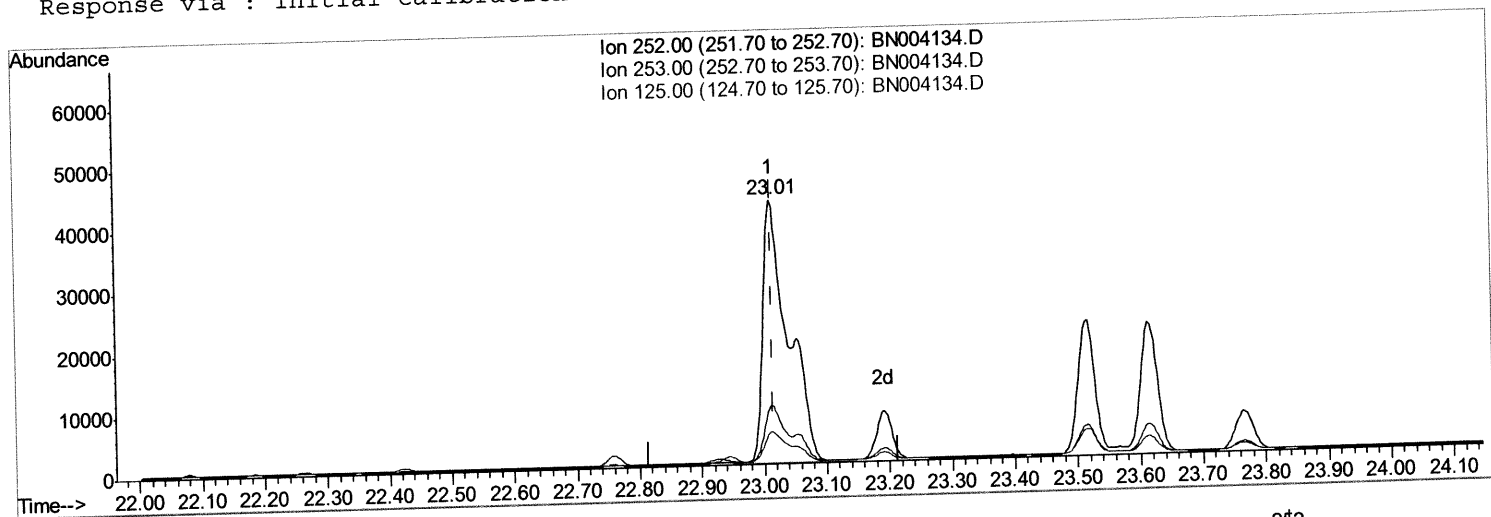

(21) Benzo(b)fluoranthene

23.013min (-0.002) 2.35ng/ul

response 120829

Ion	Exp%	Act%
252.00	100	100
253.00	23.00	22.51
125.00	11.20	12.43
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Qedit)




Data File : BN004134.D
Acq On : 20 Dec 2018 03:15
Operator : JU/SJ
Sample : J6299-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F24

Manual Integrations
APPROVED

Sohil
12/20/2018 2:03:54 PM

Quant Time: Dec 20 07:31:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

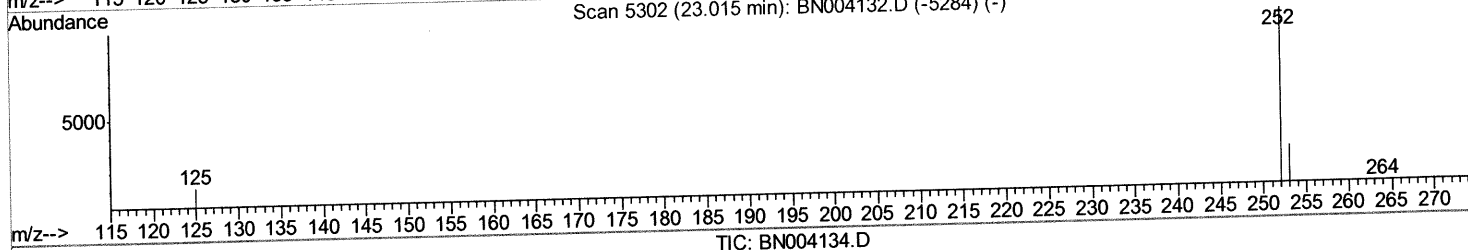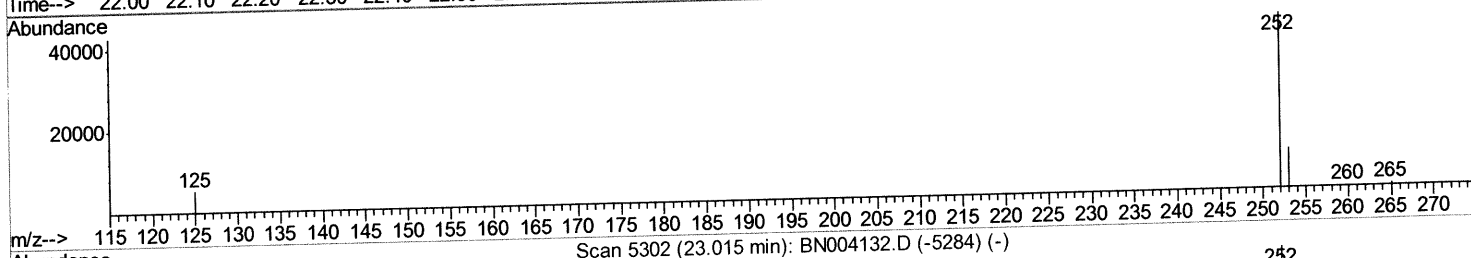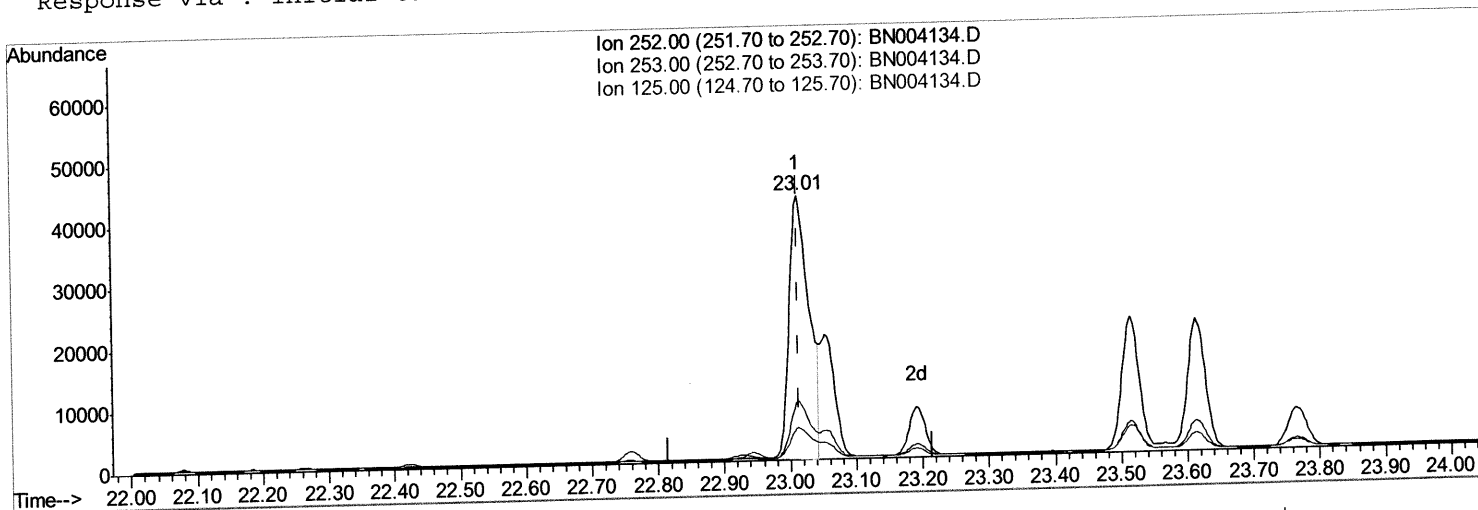

(21) Benzo(b)fluoranthene

23.013min (-0.002) 1.75ng/ul m

response 89664

Ion	Exp%	Act%
252.00	100	100
253.00	23.00	22.51
125.00	11.20	12.43
0.00	0.00	0.00

> SJ
12/20/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Qedit)




Data File : BN004134.D
Acq On : 20 Dec 2018 03:15
Operator : JU/SJ
Sample : J6299-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F24

Manual Integrations
APPROVED

Sohil
12/20/2018 2:03:54 PM

Quant Time: Dec 20 07:31:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

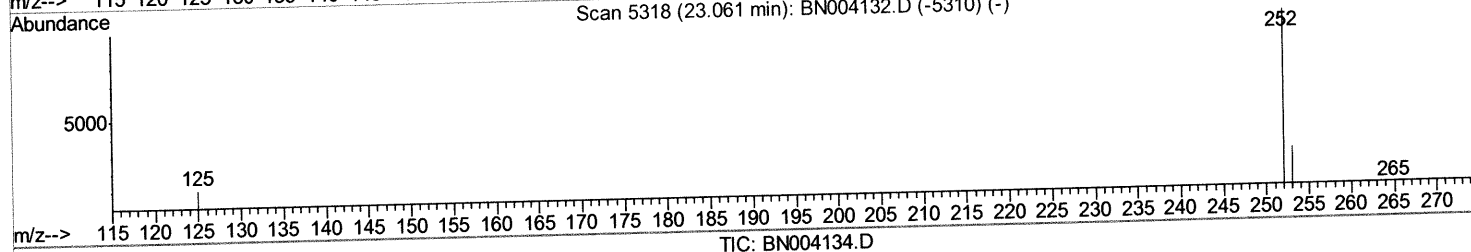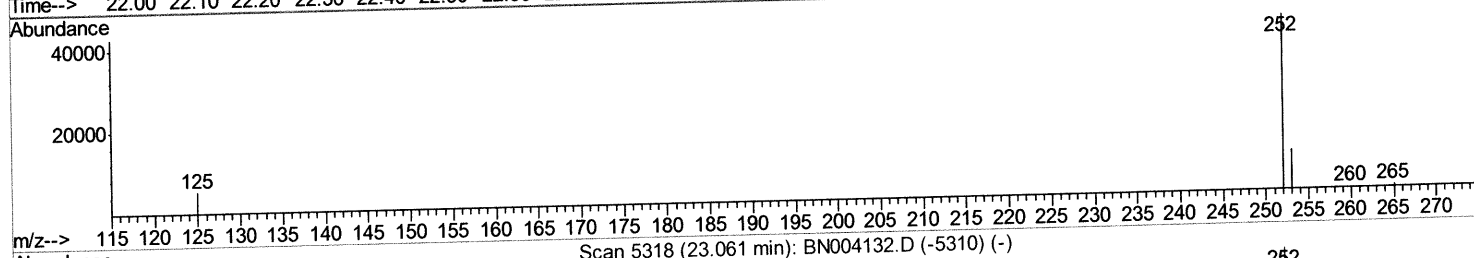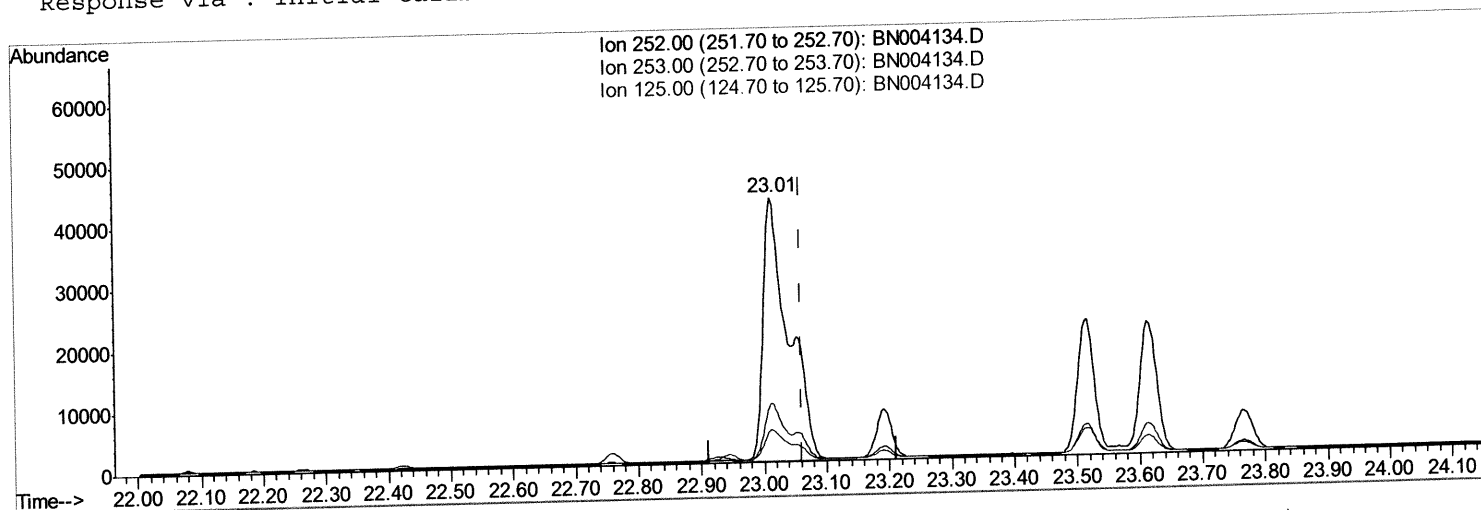

(22) Benzo(k)fluoranthene
23.013min (-0.048) 2.42ng/ul
response 120829

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	22.51
125.00	11.30	12.43
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Qedit)


Data File : BN004134.D
Acq On : 20 Dec 2018 03:15
Operator : JU/SJ
Sample : J6299-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F24

Manual Integrations
APPROVED

Sohil
12/20/2018 2:03:54 PM

Quant Time: Dec 20 07:31:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

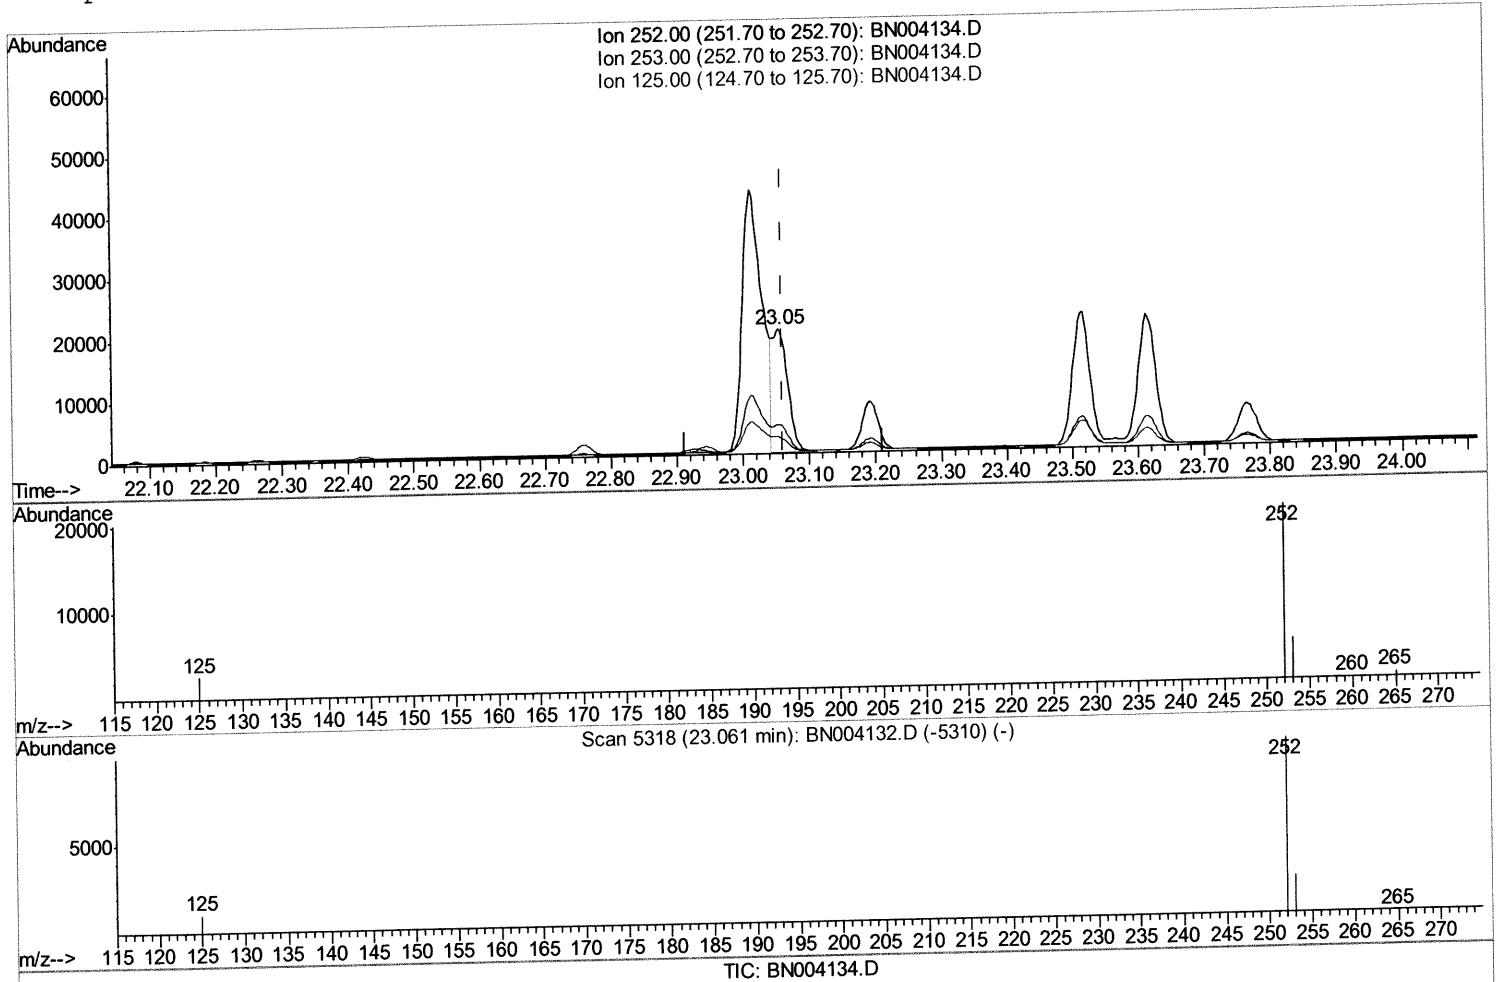

(22) Benzo(k)fluoranthene

23.054min (-0.007) 0.64ng/ul m

response 31831

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	23.50
125.00	11.30	13.31
0.00	0.00	0.00

> SJ
12/20/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Qedit)




Data File : BN004134.D
Acq On : 20 Dec 2018 03:15
Operator : JU/SJ
Sample : J6299-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F24

Manual Integrations
APPROVED

Sohil
12/20/2018 2:03:54 PM

Quant Time: Dec 20 07:31:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

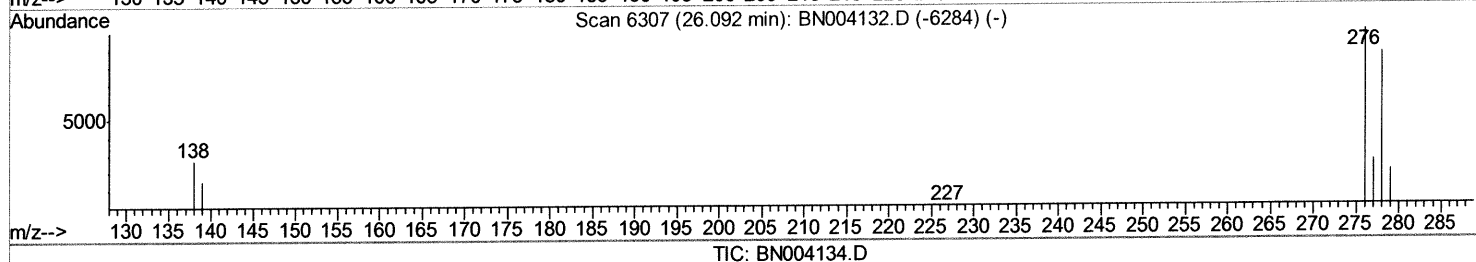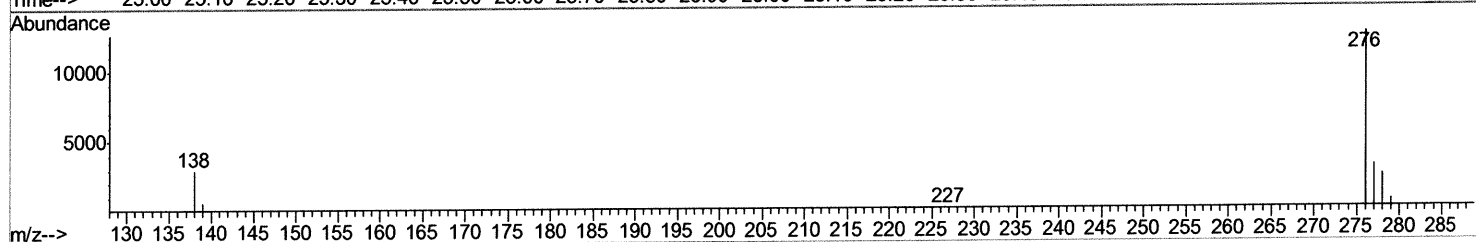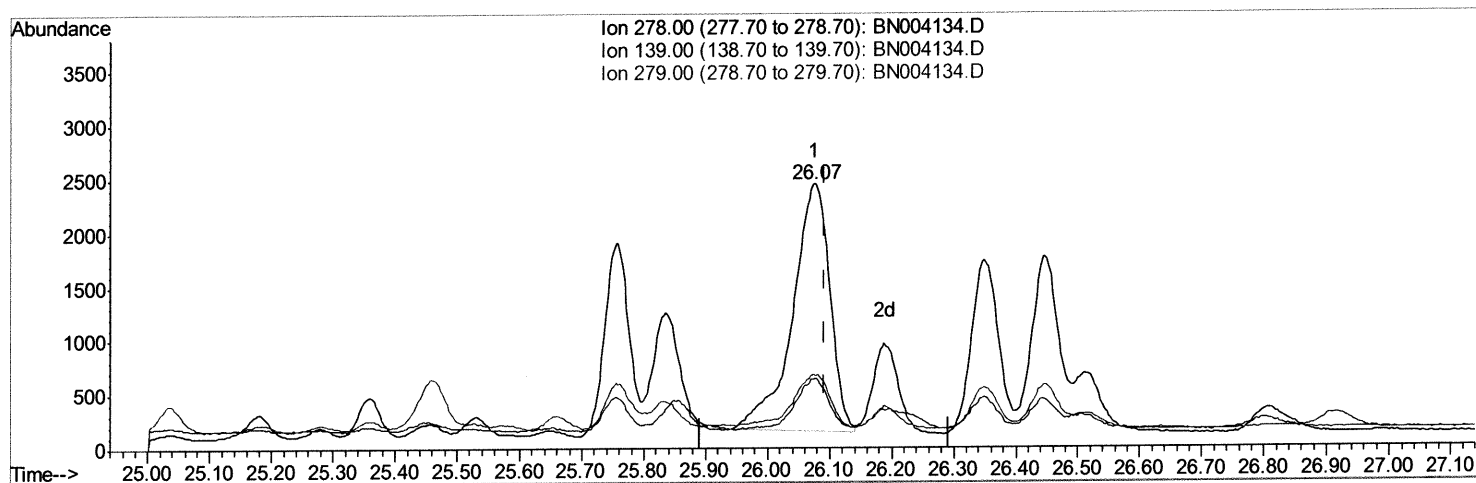

(25) Dibenzo(a,h)anthracene

26.074min (-0.018) 0.23ng/ul

response 9568

Ion	Exp%	Act%
278.00	100	100
139.00	17.80	26.04#
279.00	24.70	27.83
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Qedit)




Data File : BN004134.D
Acq On : 20 Dec 2018 03:15
Operator : JU/SJ
Sample : J6299-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F24

Manual Integrations
APPROVED

Sohil
12/20/2018 2:03:54 PM

Quant Time: Dec 20 07:31:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

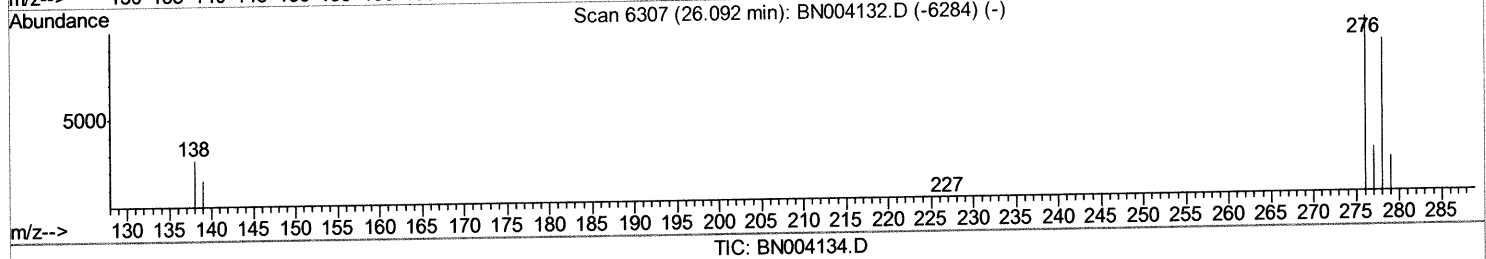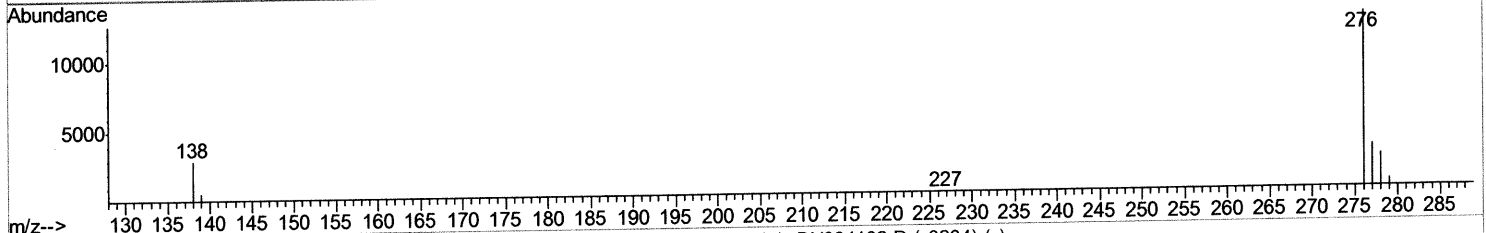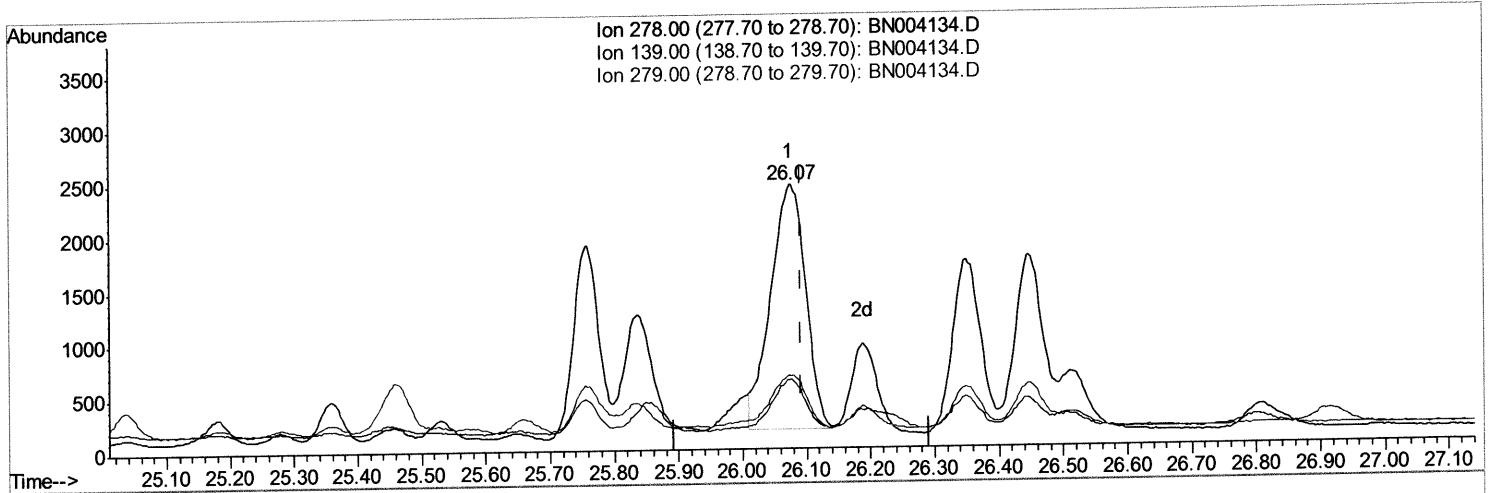

(25) Dibenzo(a,h)anthracene

26.074min (-0.018) 0.21ng/ul m

response 8656

Ion Exp% Act%

278.00 100 100

139.00 17.80 26.04#

279.00 24.70 27.83

0.00 0.00 0.00

> SJ
12/20/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (QT Reviewed)

Data File : BN004134.D
Acq On : 20 Dec 2018 03:15
Operator : JU/SJ
Sample : J6299-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F24

Manual Integrations
APPROVED

Sohil
12/20/2018 2:03:54 PM

Quant Time: Dec 20 07:32:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	1471	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	7734	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	4747	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	12457m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	13337m	0.40	ng/ul	0.00
20) Perylene-d12	23.71	264	12411m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.22	152	2045	0.17	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	6562m	0.18	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
7) Acenaphthylene	14.19	152	14824	0.694	ng/ul	99
12) Phenanthrene	17.25	178	3927m	0.096	ng/ul	
13) Anthracene	17.35	178	13761m	0.410	ng/ul	
15) Fluoranthene	19.27	202	64591m	1.338	ng/ul	
17) Pyrene	19.63	202	72300	1.511	ng/ul	95
18) Benzo(a)anthracene	21.38	228	46906	1.114	ng/ul	98
19) Chrysene	21.43	228	48826	1.013	ng/ul	98
21) Benzo(b)fluoranthene	23.01	252	89664m	1.746	ng/ul	
22) Benzo(k)fluoranthene	23.05	252	31831m	0.636	ng/ul	
23) Benzo(a)pyrene	23.61	252	39668	0.892	ng/ul	98
24) Indeno(1,2,3-cd)pyrene	26.07	276	36565	0.717	ng/ul#	95
25) Dibenzo(a,h)anthracene	26.07	278	8656m	0.211	ng/ul	
26) Benzo(g,h,i)perylene	26.80	276	26348	0.595	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

57
12/20/18