

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Data File : BN004138.D
Acq On : 20 Dec 2018 05:35
Operator : JU/SJ
Sample : J6299-12
Misc :
ALS Vial : 35
Sample Multiplier: 1


Quantitation Report (QT Reviewed)

Instrument :
BNA_N
ClientSampleId :
F9F39

Manual Integrations
APPROVED

Sohil
12/20/2018 2:04:04 PM

Quant Time: Dec 20 07:47:49 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

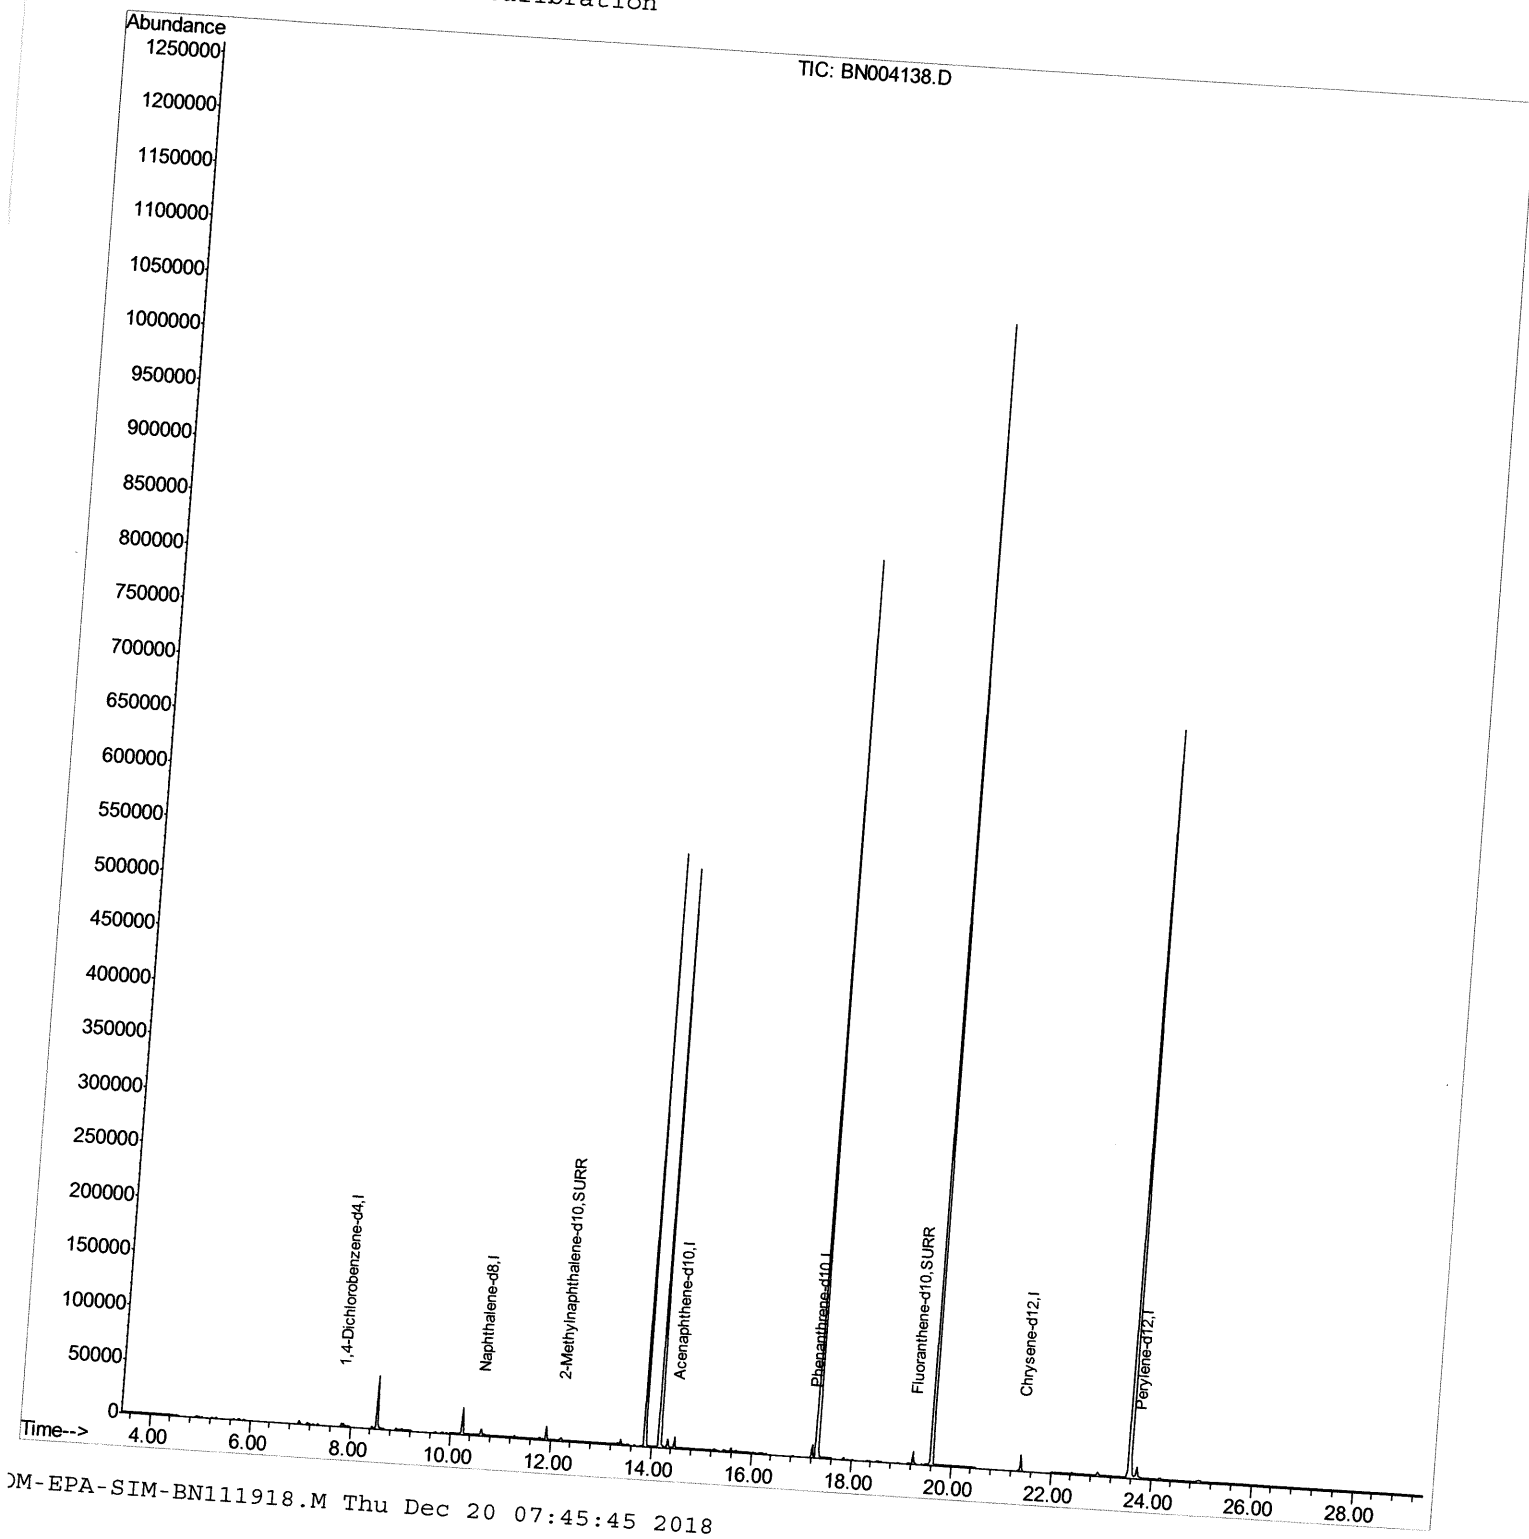




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
 Data File : BN004138.D
 Acq On : 20 Dec 2018 05:35
 Operator : JU/SJ
 Sample : J6299-12
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9F39

Manual Integrations
 APPROVED

Sohil
 12/20/2018 2:04:04 PM

Quant Time: Dec 20 07:21:00 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Qlast Update : Thu Dec 20 07:15:48 2018
 Response via : Initial Calibration

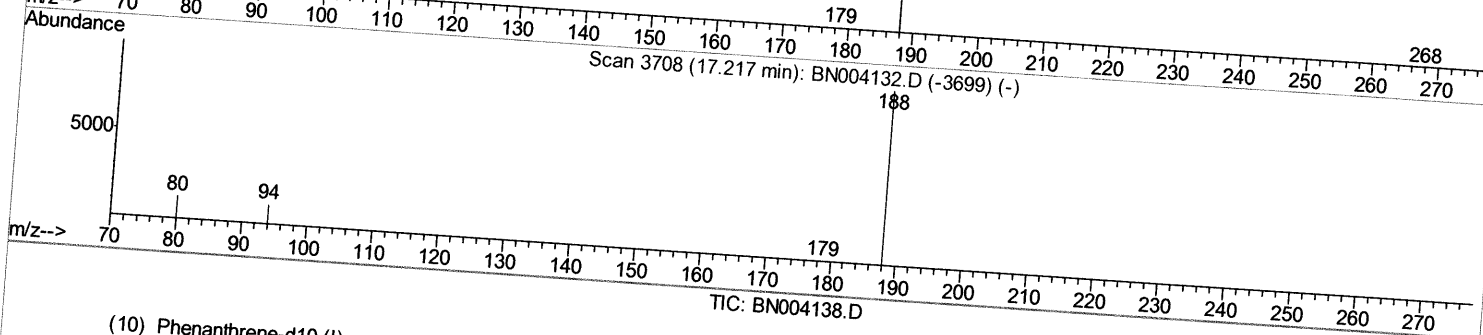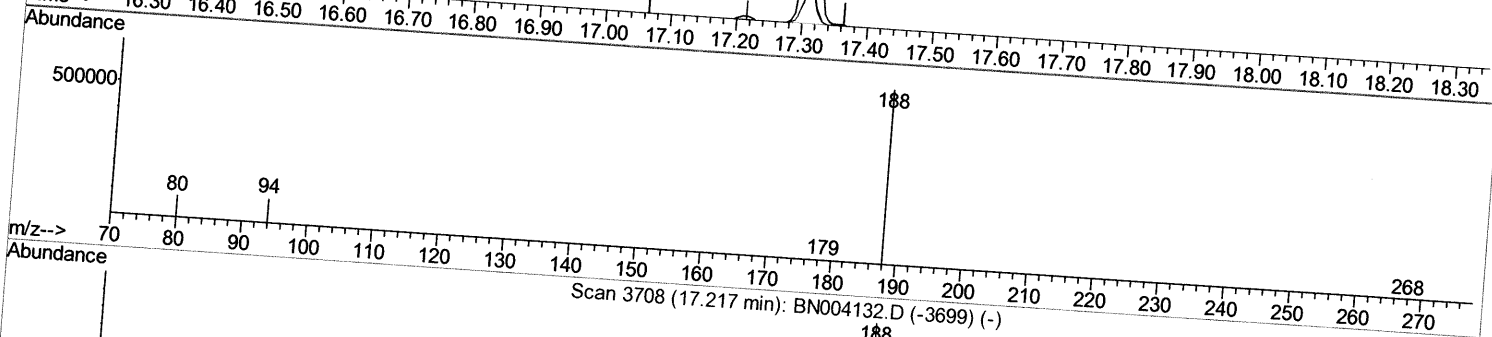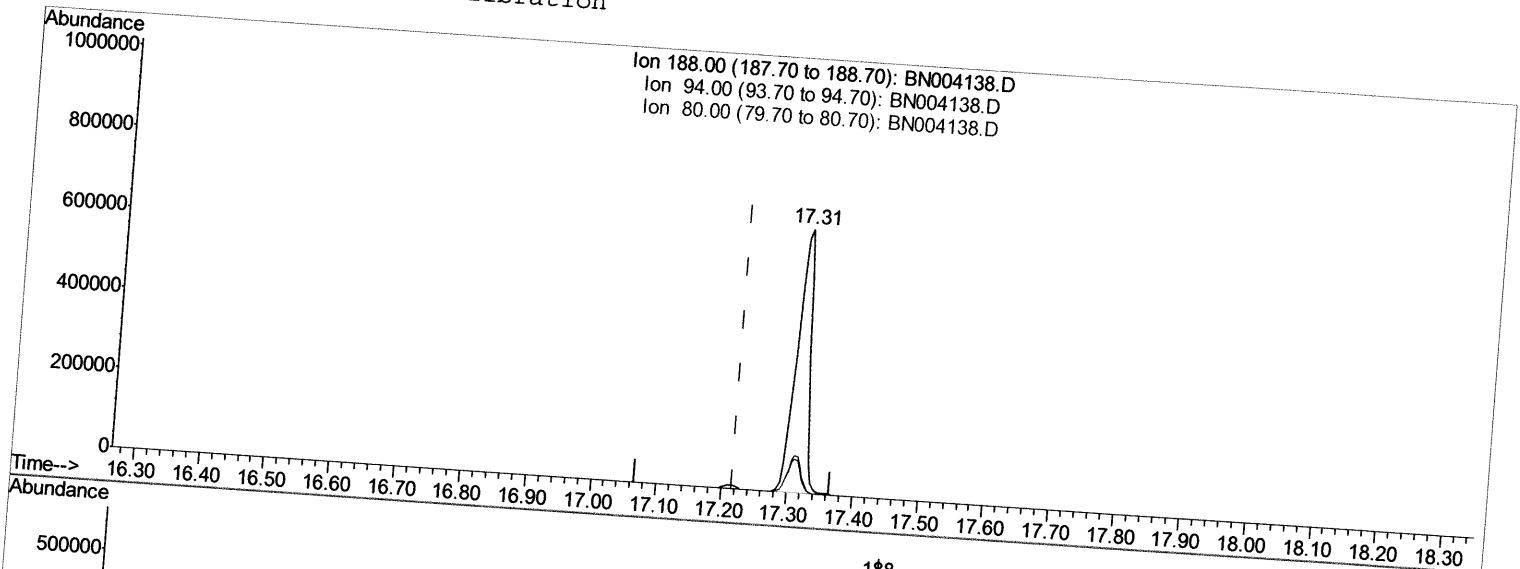

(10) Phenanthrene-d10 (I)
 17.314min (+0.097) 0.40ng/ul

response 914595

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	13.71#
80.00	11.60	12.21
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Qedit)




Instrument :
BNA_N
ClientSampleId :
F9F39

Manual Integrations
APPROVED

Sohil
12/20/2018 2:04:04 PM

Data File : BN004138.D
Acq On : 20 Dec 2018 05:35
Operator : JU/SJ
Sample : J6299-12
Misc :
ALS Vial : 35 Sample Multiplier: 1

Quant Time: Dec 20 07:21:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

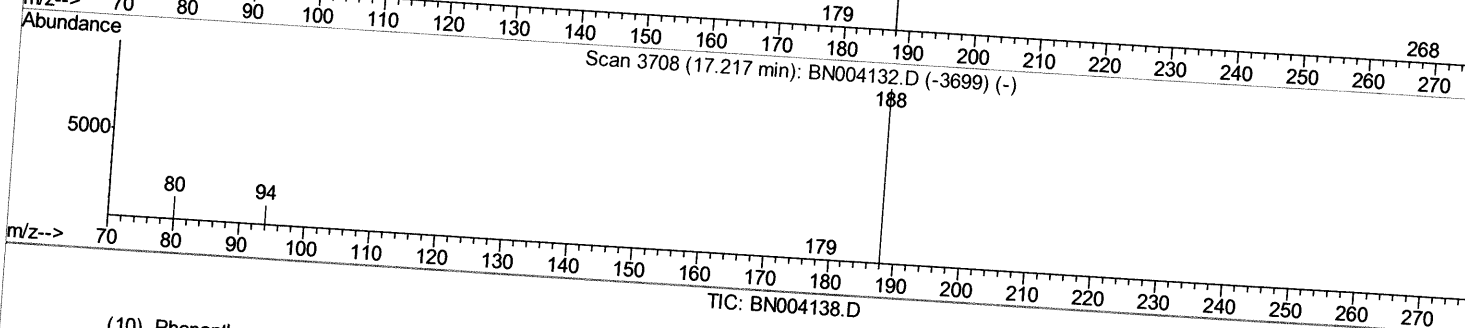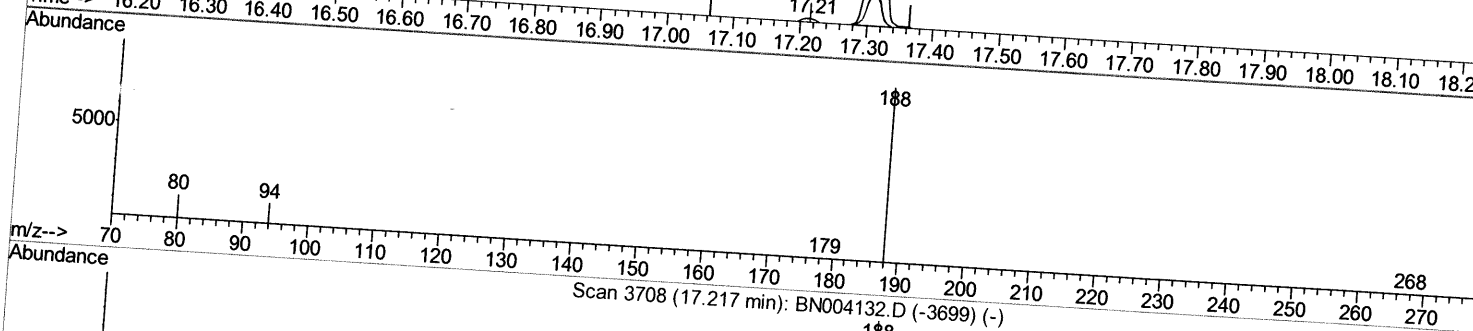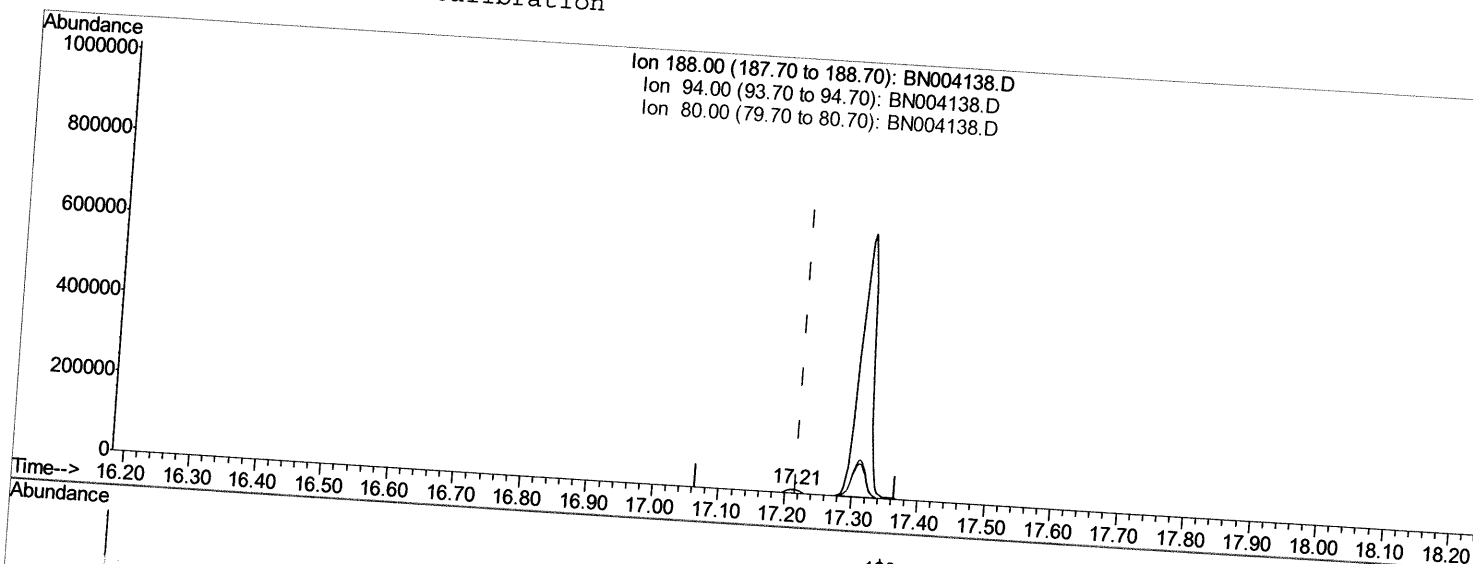

(10) Phenanthrene-d10 (I)

17.213min (-0.004) 0.40ng/ul m

response 12769

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	12.04
80.00	11.60	13.58
0.00	0.00	0.00

> SJ
12/20/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Qedit)




Data File : BN004138.D
Acq On : 20 Dec 2018 05:35
Operator : JU/SJ
Sample : J6299-12
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F39

Manual Integrations
APPROVED

Sohil
12/20/2018 2:04:04 PM

Quant Time: Dec 20 07:46:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

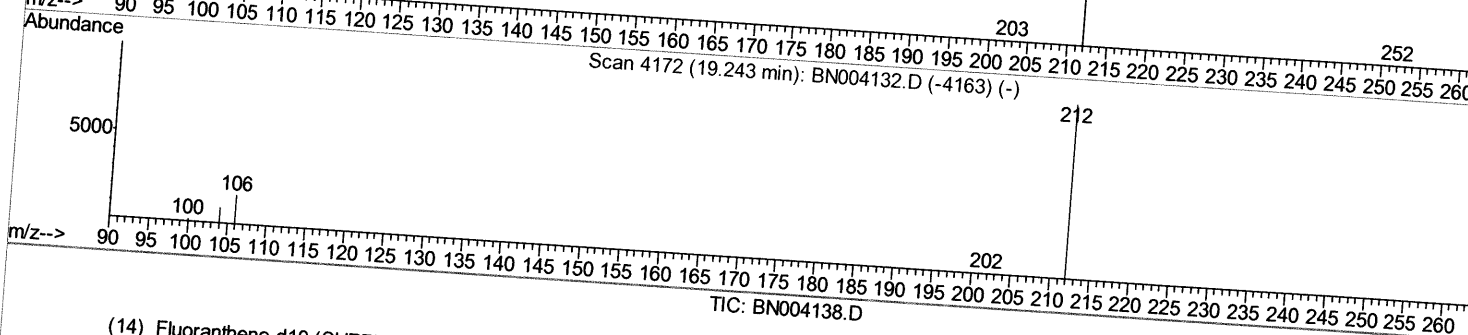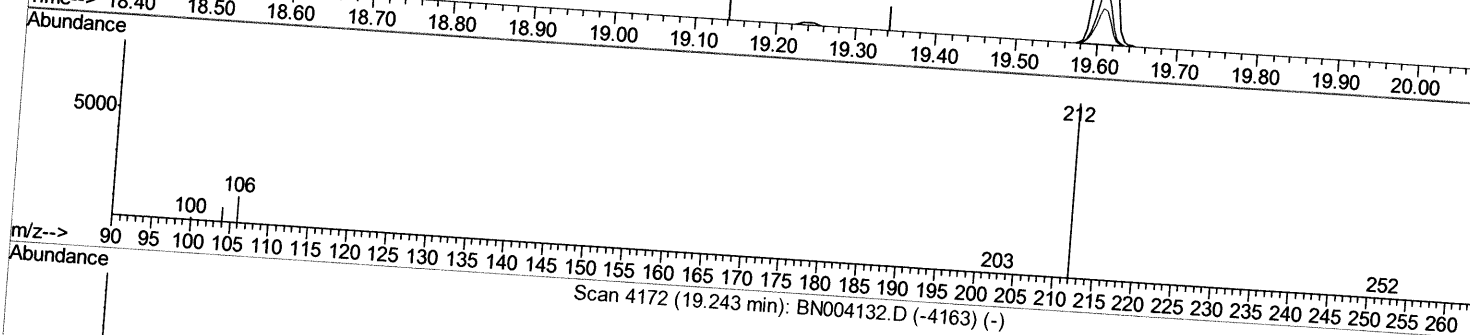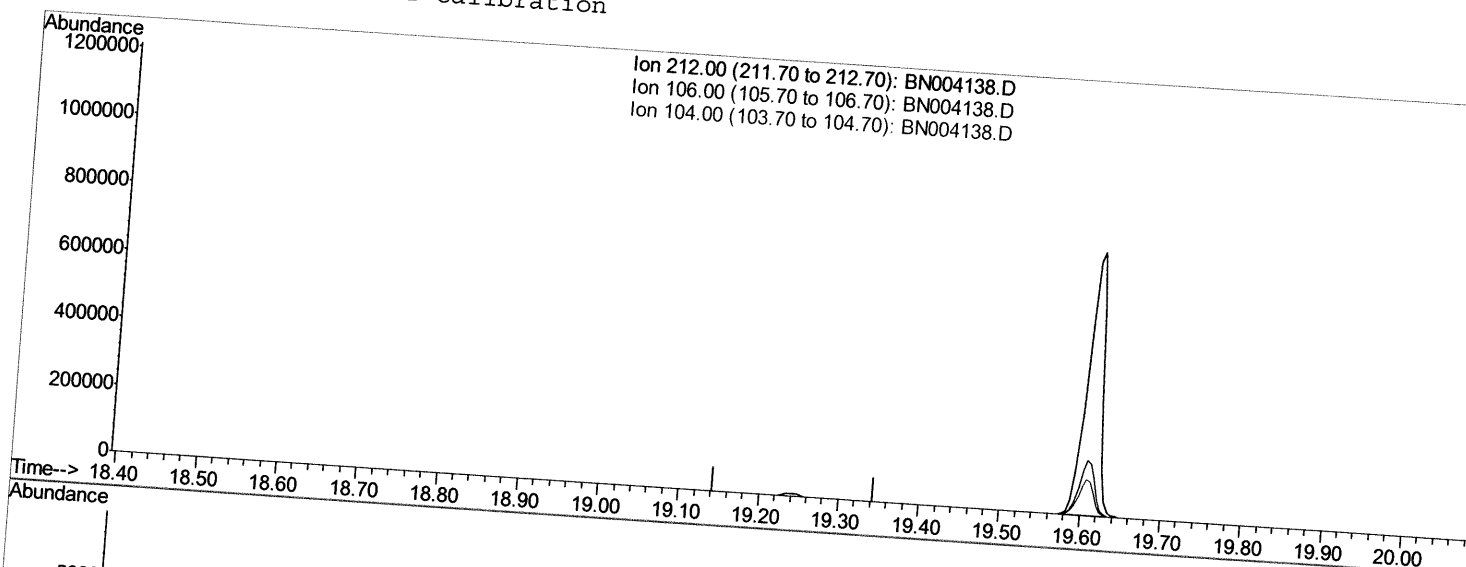

(14) Fluoranthene-d10 (SURR)

19.243min (-19.243) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Data File : BN004138.D
Acq On : 20 Dec 2018 05:35
Operator : JU/SJ
Sample : J6299-12
Misc :
ALS Vial : 35 Sample Multiplier: 1




Quantitation Report (Qedit)

Instrument :
BNA_N
ClientSampleId :
F9F39

Manual Integrations
APPROVED

Sohil
12/20/2018 2:04:04 PM

Quant Time: Dec 20 07:46:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

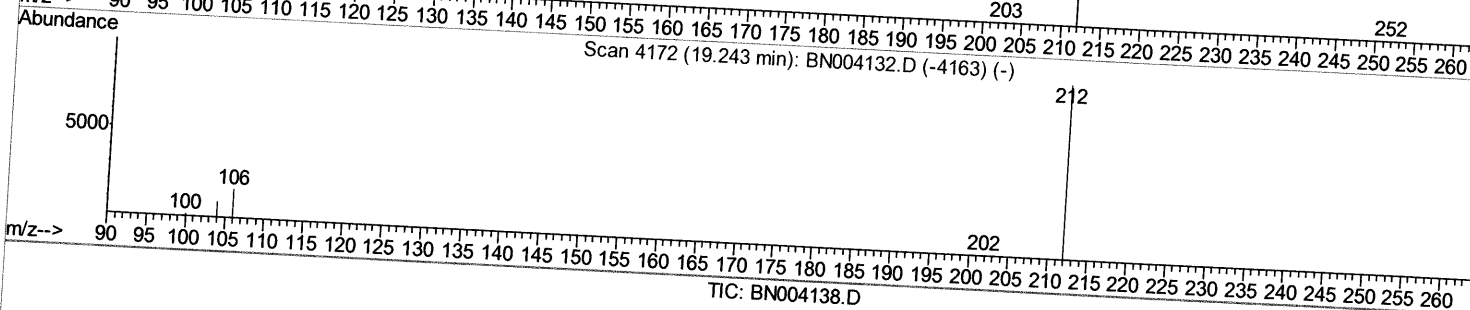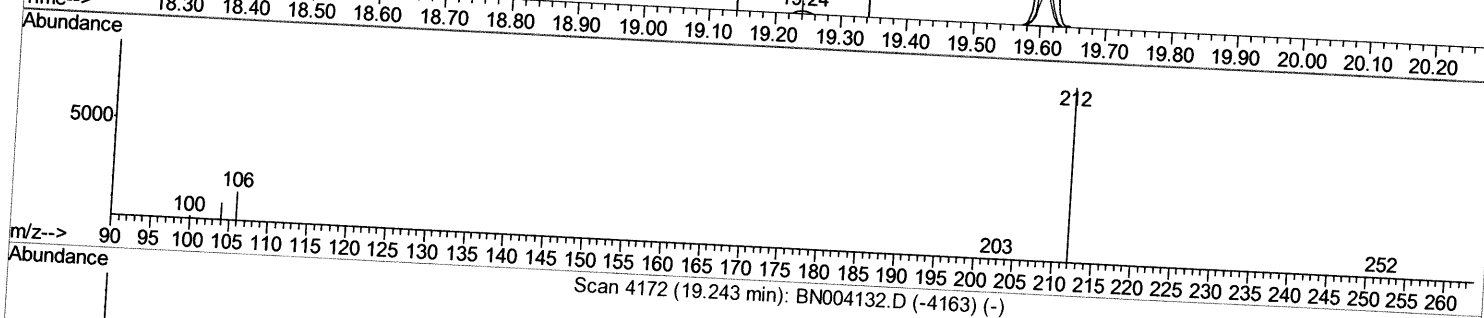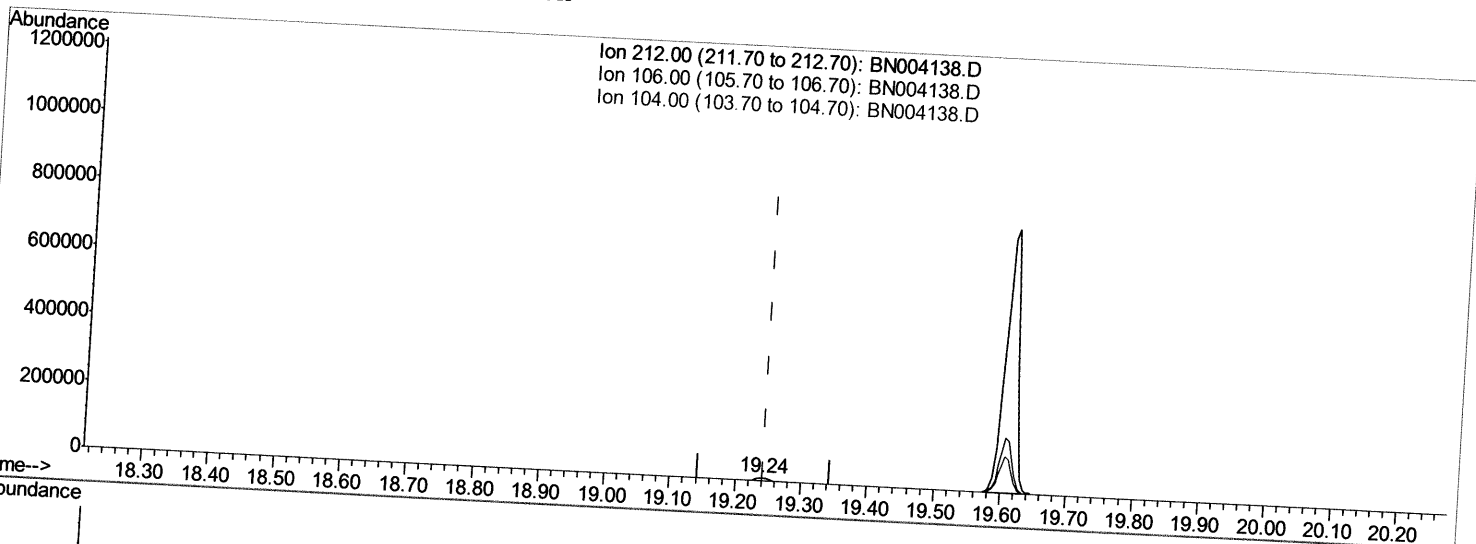

(14) Fluoranthene-d10 (SURR)

19.239min (-0.004) 0.31ng/ul m

response 11659

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

> SJ
12/20/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Qedit)

Instrument :
BNA_N
ClientSampleId :
F9F39


Manual Integrations
APPROVED

Sohil
12/20/2018 2:04:04 PM

Data File : BN004138.D
Acq On : 20 Dec 2018 05:35
Operator : JU/SJ
Sample : J6299-12
Misc :
ALS Vial : 35 Sample Multiplier: 1

Quant Time: Dec 20 07:46:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

Ion 240.00 (239.70 to 240.70): BN004138.D
Ion 120.00 (119.70 to 120.70): BN004138.D
Ion 236.00 (235.70 to 236.70): BN004138.D

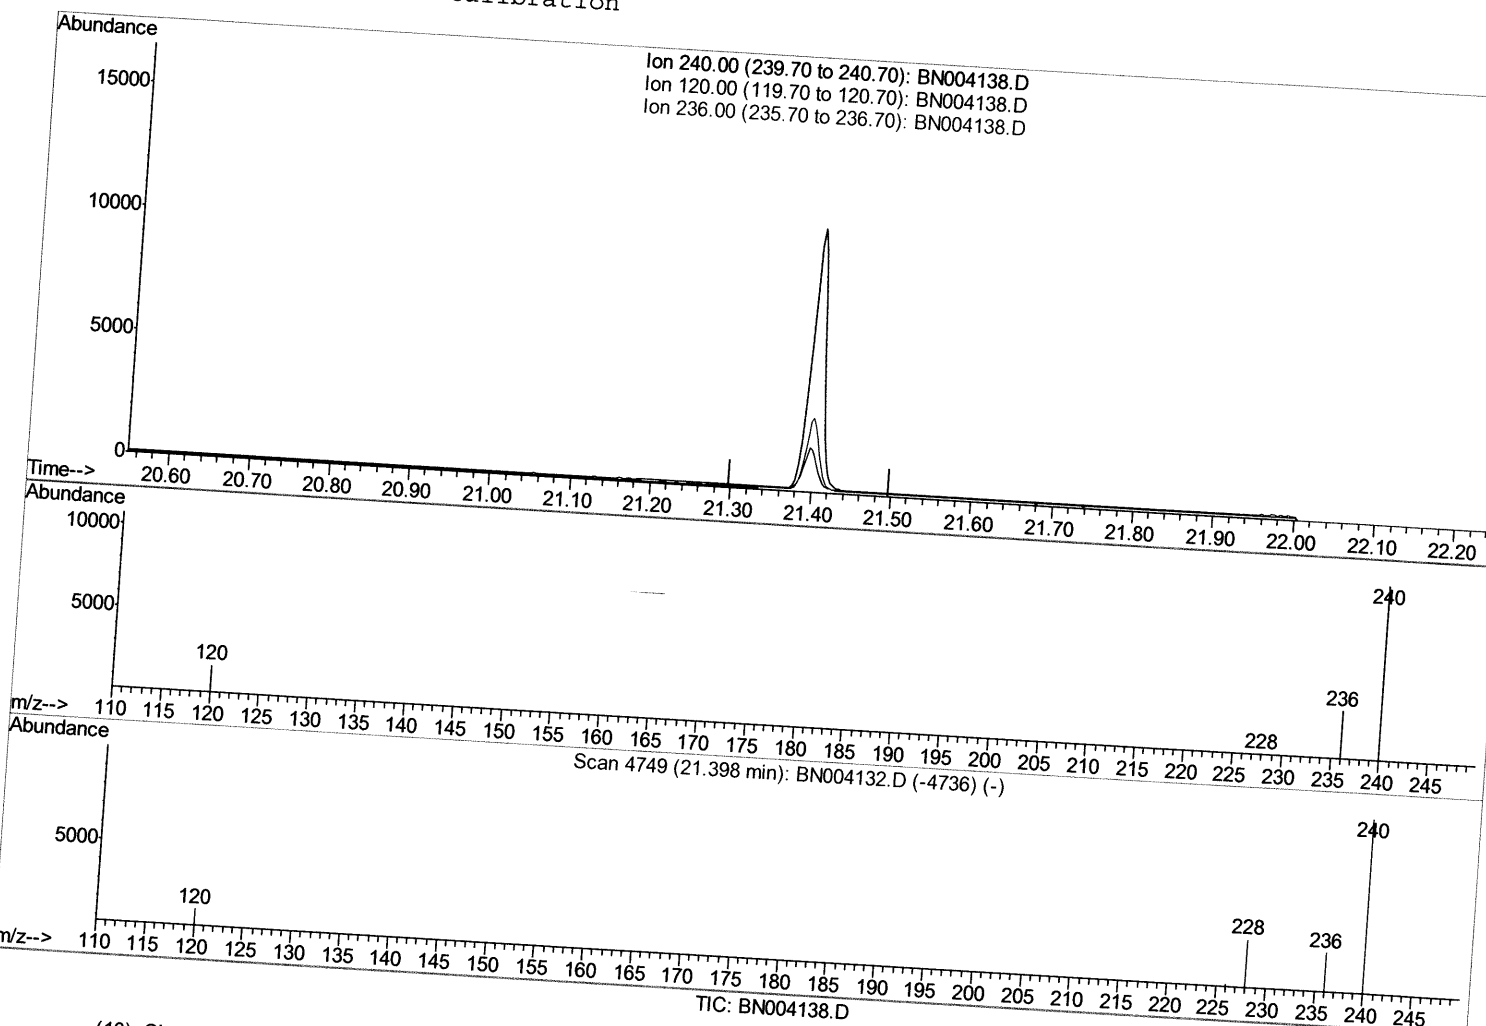

(16) Chrysene-d12 (I)

21.398min (-21.398) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Data File : BN004138.D
Acq On : 20 Dec 2018 05:35
Operator : JU/SJ
Sample : J6299-12
Misc :
ALS Vial : 35 Sample Multiplier: 1




Quantitation Report (Qedit)

Instrument :
BNA_N
ClientSampleId :
F9F39

Manual Integrations
APPROVED

Sohil
12/20/2018 2:04:04 PM

Quant Time: Dec 20 07:46:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

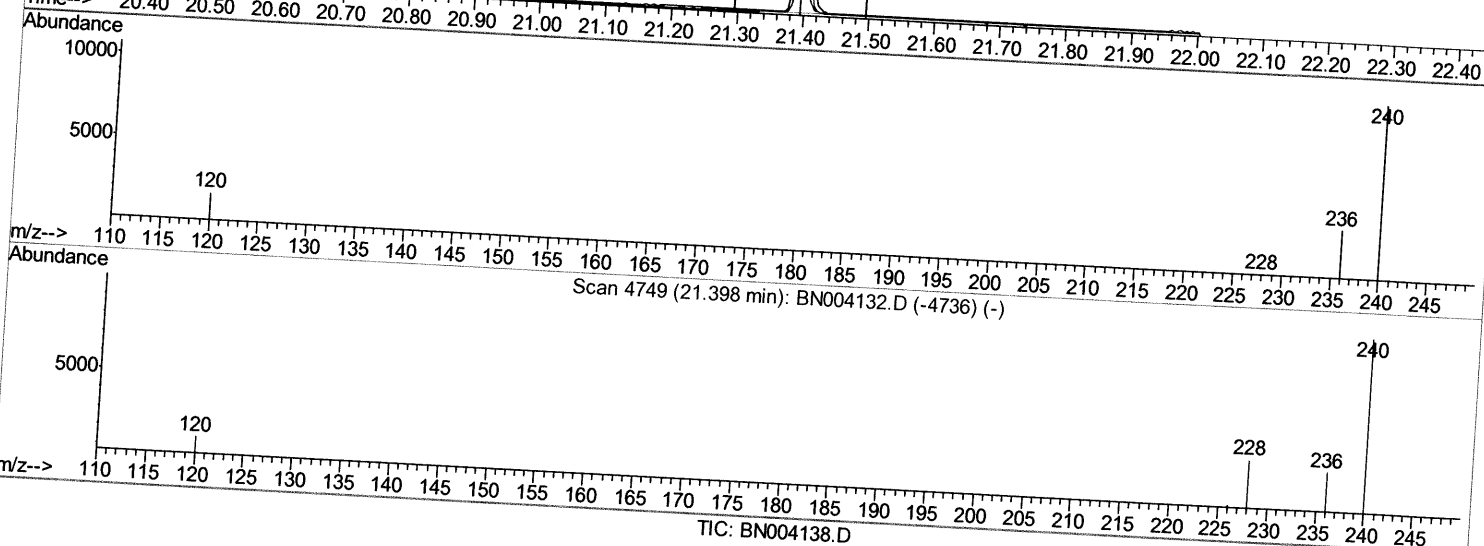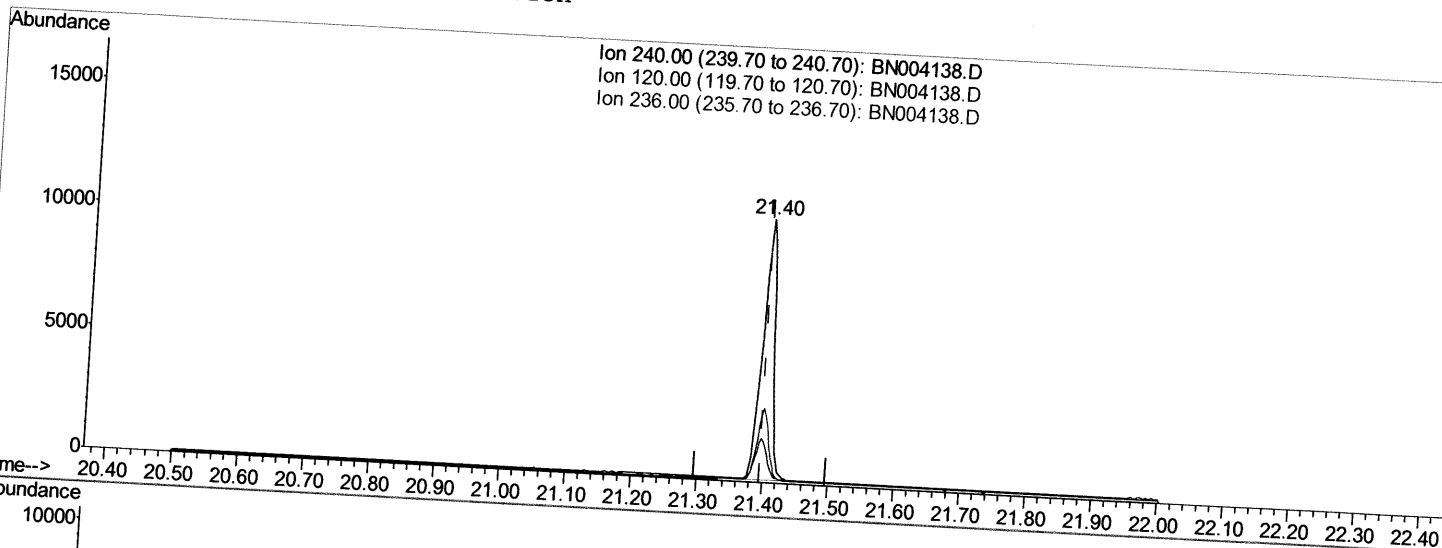

(16) Chrysene-d12 (I)

21.400min (+0.001) 0.40ng/ul m

response 12864

> $\frac{5J}{12/20/18}$

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	15.97
236.00	27.60	28.10
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Data File : BN004138.D Quantitation Report (Qedit)

Instrument :
BNA_N
ClientSampled :
F9F39

Manual Integrations
APPROVED

Sohil
12/20/2018 2:04:04 PM

Acq On : 20 Dec 2018 05:35
Operator : JU/SJ
Sample : J6299-12
Misc :
ALS Vial : 35 Sample Multiplier: 1
Quant Time: Dec 20 07:47:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

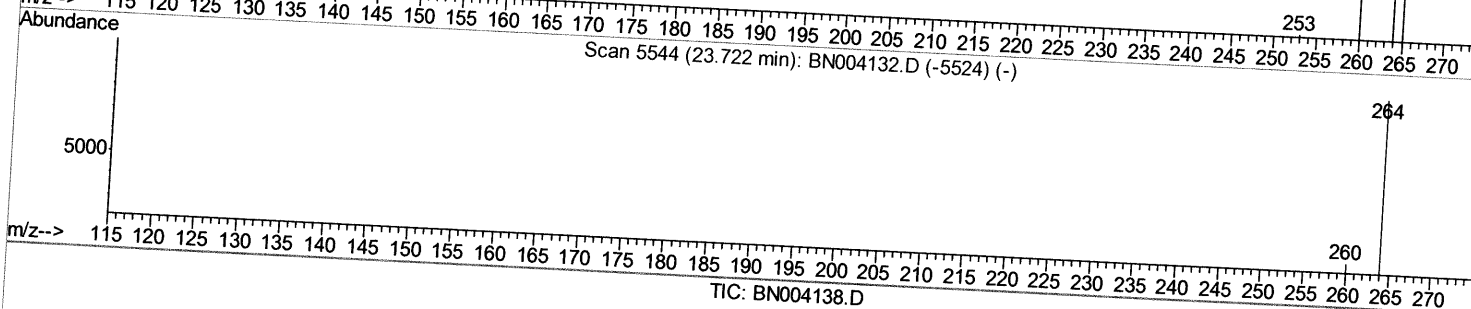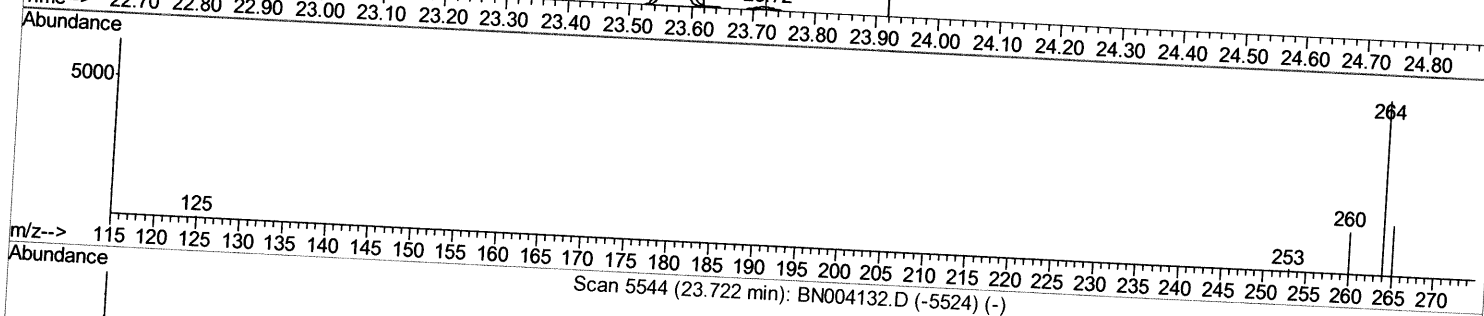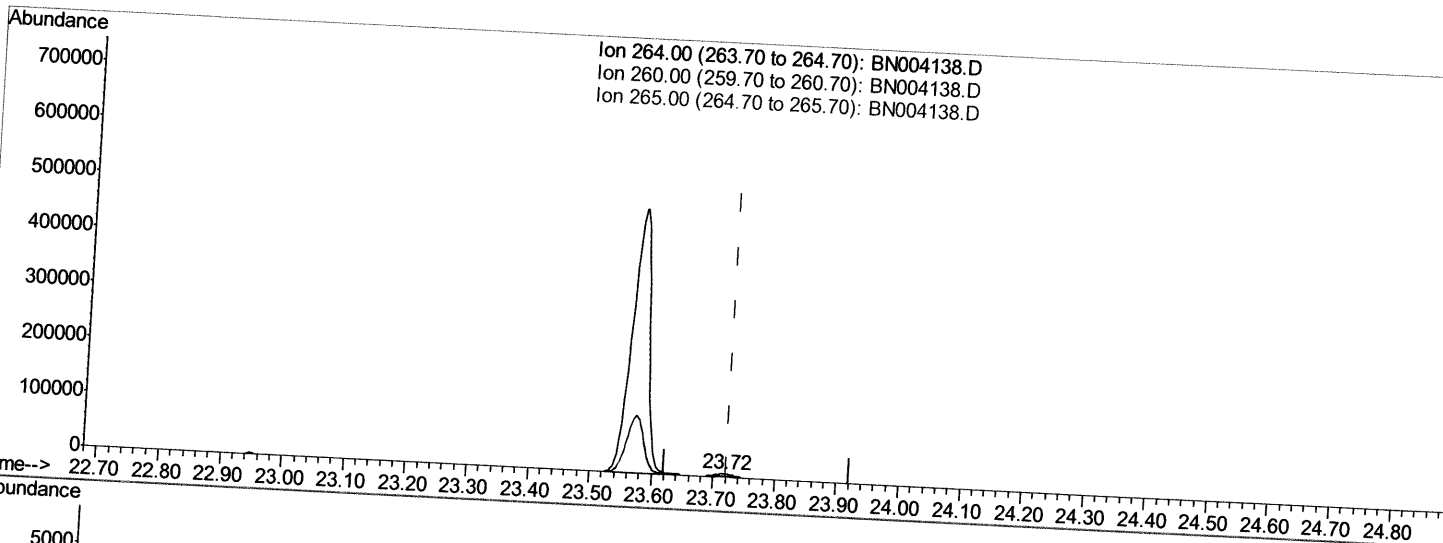

(20) Perylene-d12 (I)

23.718min (-0.004) 0.40ng/ul

response 13206

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	26.45
265.00	33.50	30.78
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (Qedit)




Instrument :
BNA_N
ClientSampleId :
F9F39

Manual Integrations
APPROVED

Sohil
12/20/2018 2:04:04 PM

Data File : BN004138.D
Acq On : 20 Dec 2018 05:35
Operator : JU/SJ
Sample : J6299-12
Misc :
ALS Vial : 35 Sample Multiplier: 1

Quant Time: Dec 20 07:47:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

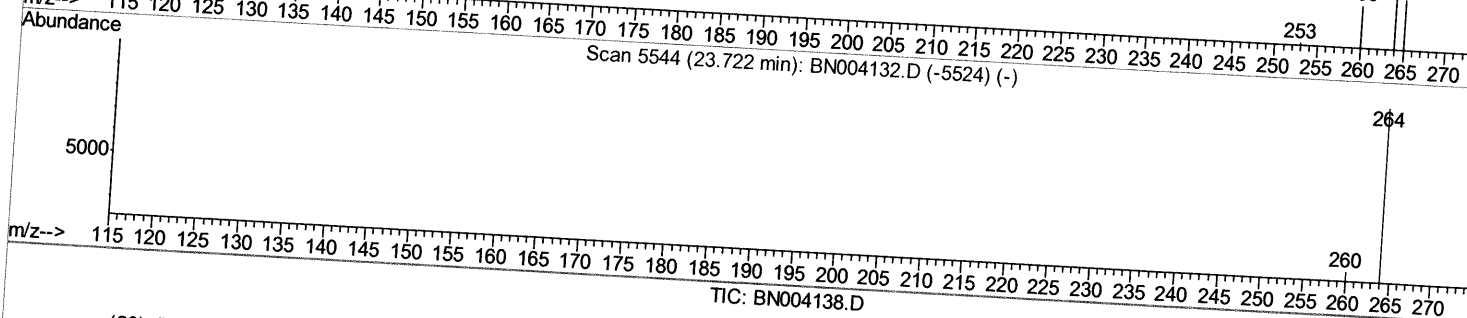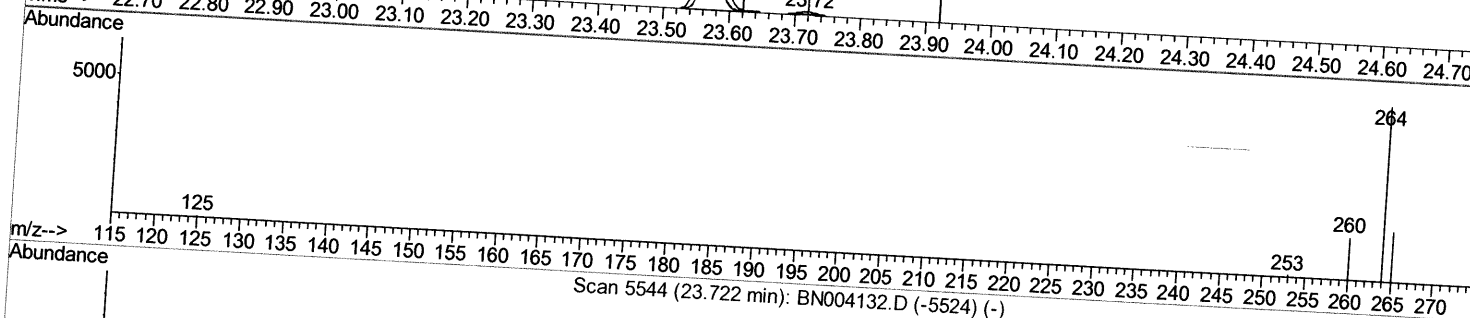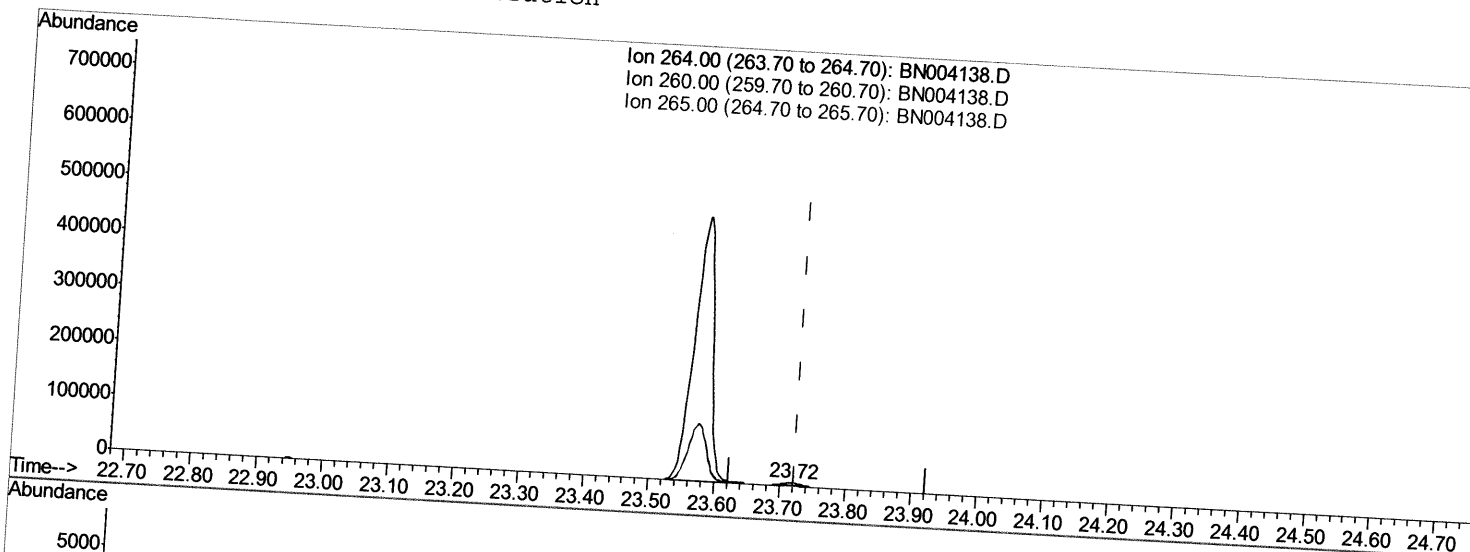

(20) Perylene-d12 (I)

23.718min (-0.004) 0.40ng/ul m

response 11186

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	26.45
265.00	33.50	30.78
0.00	0.00	0.00

> SJ
12/20/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121918\
Quantitation Report (QT Reviewed)

Instrument :
BNA_N
ClientSampleId :
F9F39

Manual Integrations
APPROVED

Sohil
12/20/2018 2:04:04 PM

Data File : BN004138.D
Acq On : 20 Dec 2018 05:35
Operator : JU/SJ
Sample : J6299-12
Misc :
ALS Vial : 35 Sample Multiplier: 1

Quant Time: Dec 20 07:47:49 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 07:15:48 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	1488	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	7733	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	5118	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	12769m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	12864m	0.40	ng/ul	0.00
20) Perylene-d12	23.72	264	11186m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	3699	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	11659m	0.31	ng/ul	0.00
Target Compounds						

Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ
12/20/18