
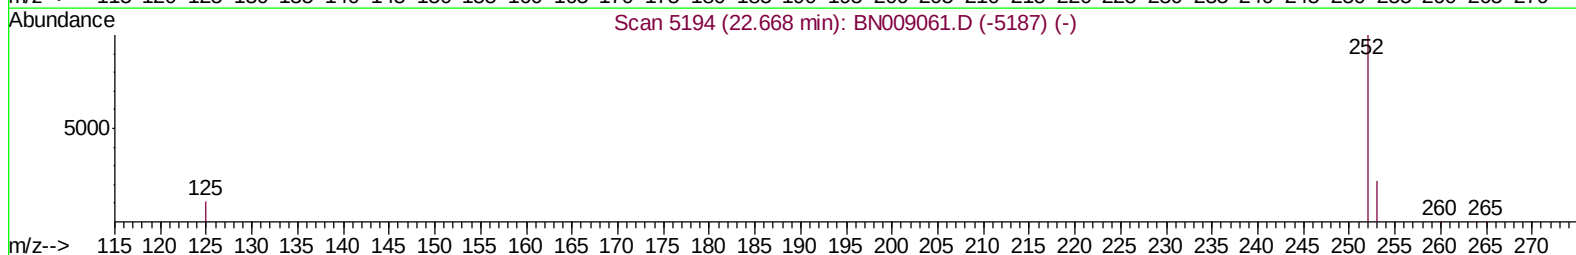
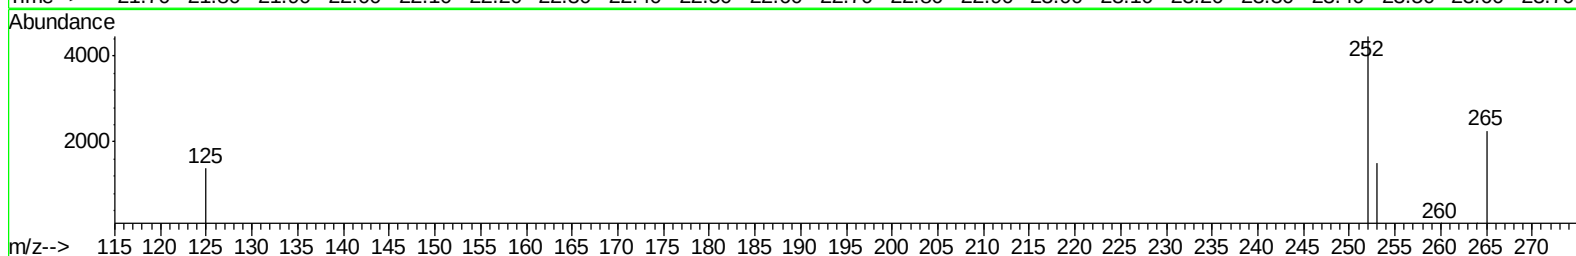


Data File : BN009071.D  
Acq On : 20 Dec 2019 16:53  
Operator : JU  
Sample : K6171-11DL 5X  
Misc :  
ALS Vial : 43 Sample Multiplier: 1

Quant Time: Dec 20 22:58:31 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-SIM-BN121619.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 20 22:55:30 2019  
Response via : Initial Calibration

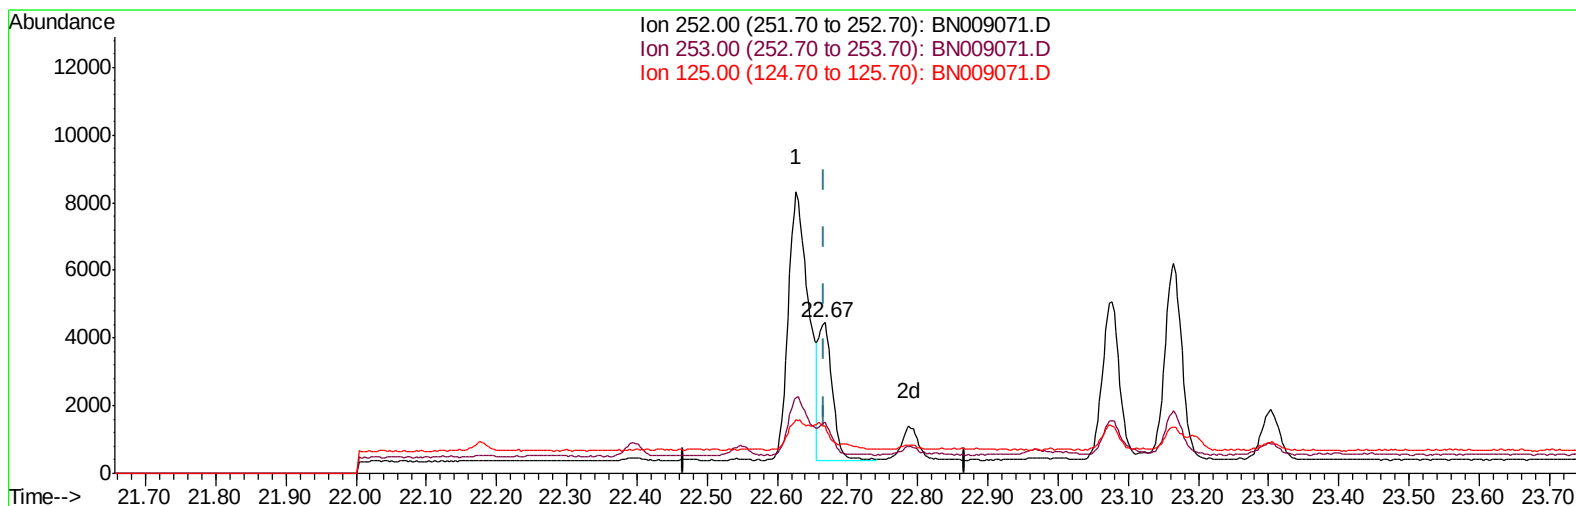

TIC: BN009071.D

(22) Benzo(k)fluoranthene

22.668min (-0.000) 0.15ng/ul m

response 5644

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 24.20 | 33.71# |
| 125.00 | 15.50 | 31.08# |
| 0.00   | 0.00  | 0.00   |