
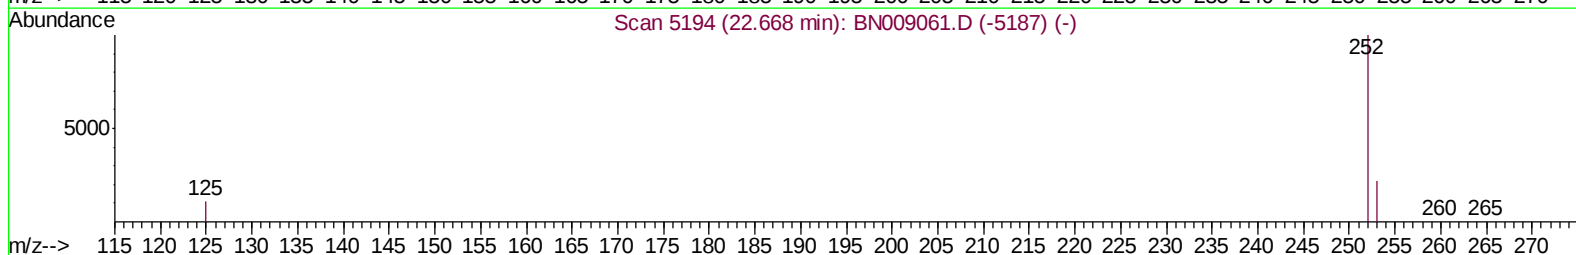
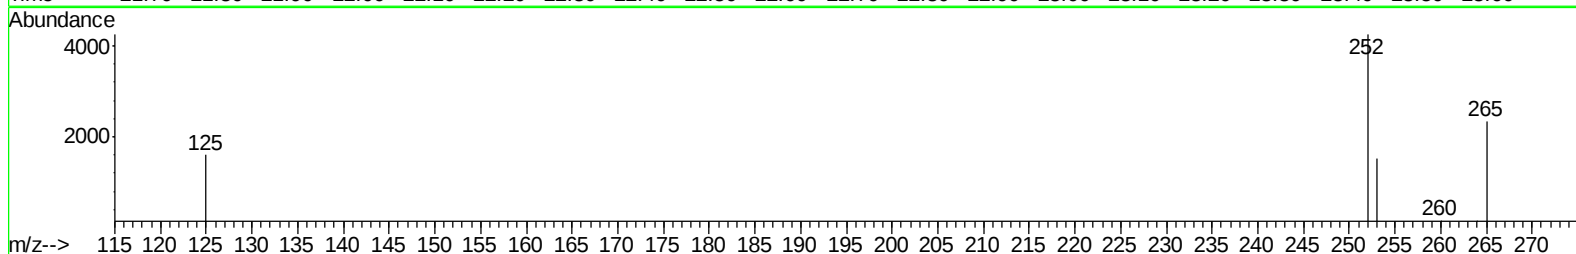


Data File : BN009072.D
Acq On : 20 Dec 2019 17:29
Operator : JU
Sample : K6171-12DL 5X
Misc :
ALS Vial : 44 Sample Multiplier: 1

Quant Time: Dec 20 22:58:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 20 22:55:30 2019
Response via : Initial Calibration

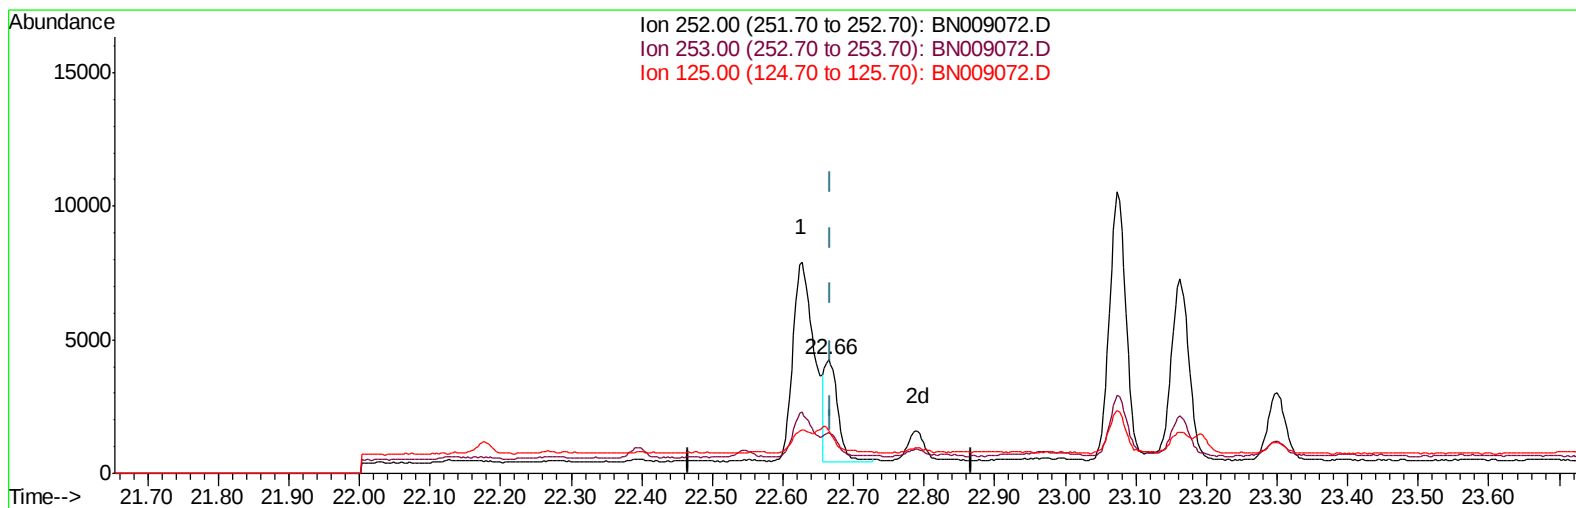

TIC: BN009072.D

(22) Benzo(k)fluoranthene

22.665min (-0.003) 0.13ng/ul m

response 5133

Ion	Exp%	Act%
252.00	100	100
253.00	24.20	35.62#
125.00	15.50	37.66#
0.00	0.00	0.00