
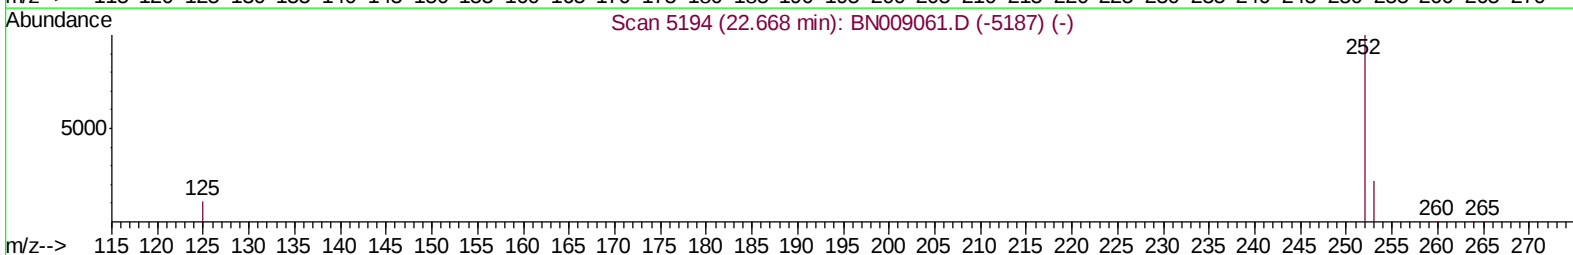
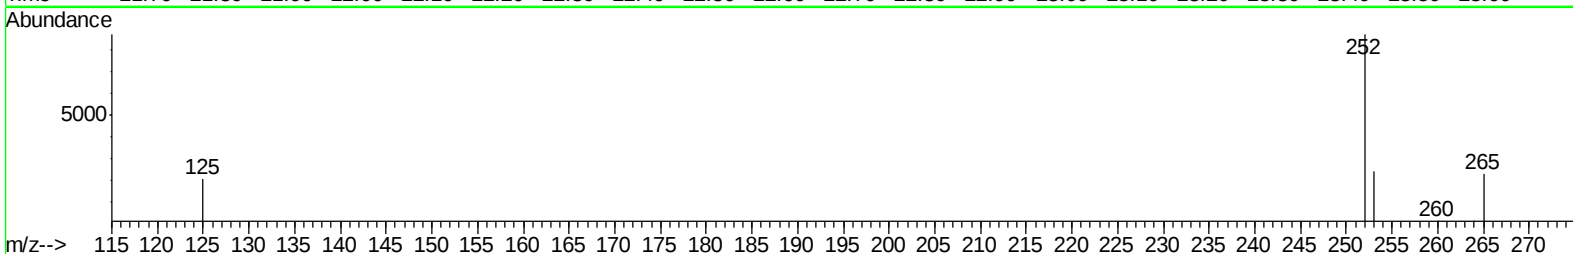


Data File : BN009074.D
Acq On : 20 Dec 2019 18:40
Operator : JU
Sample : K6171-15DL 5X
Misc :
ALS Vial : 46 Sample Multiplier: 1

Quant Time: Dec 20 22:59:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 20 22:55:30 2019
Response via : Initial Calibration

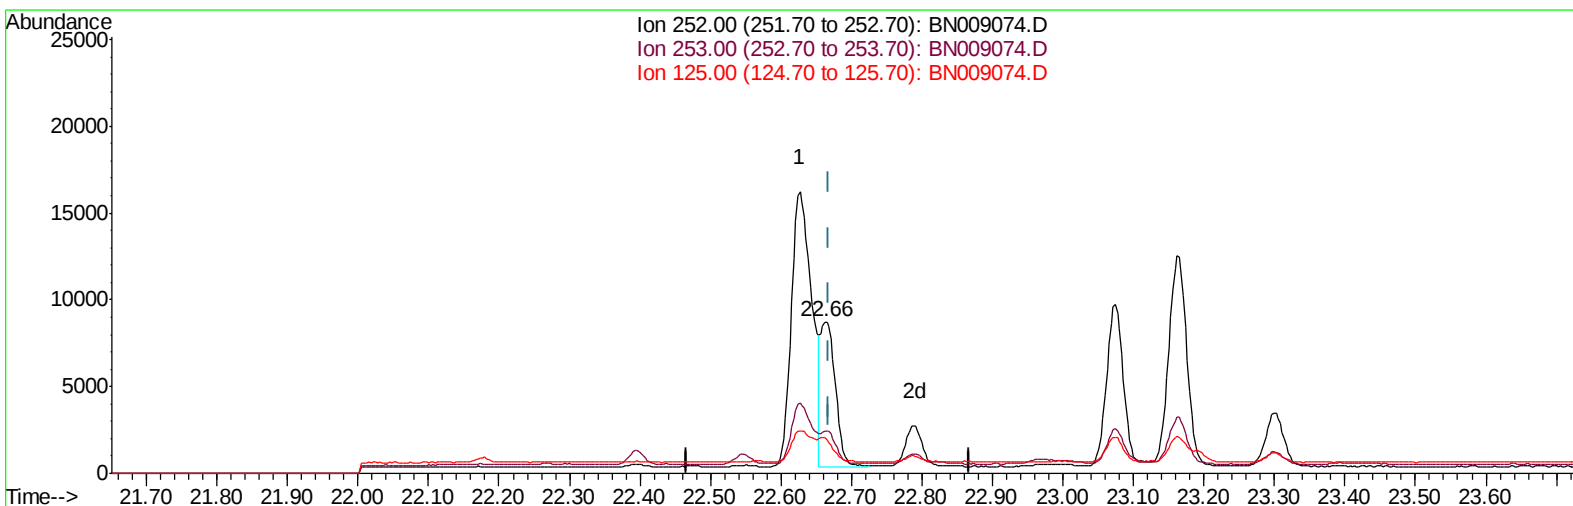

TIC: BN009074.D

(22) Benzo(k)fluoranthene

22.662min (-0.006) 0.29ng/ul m

response 12349

Ion	Exp%	Act%
252.00	100	100
253.00	24.20	27.87
125.00	15.50	23.41#
0.00	0.00	0.00