
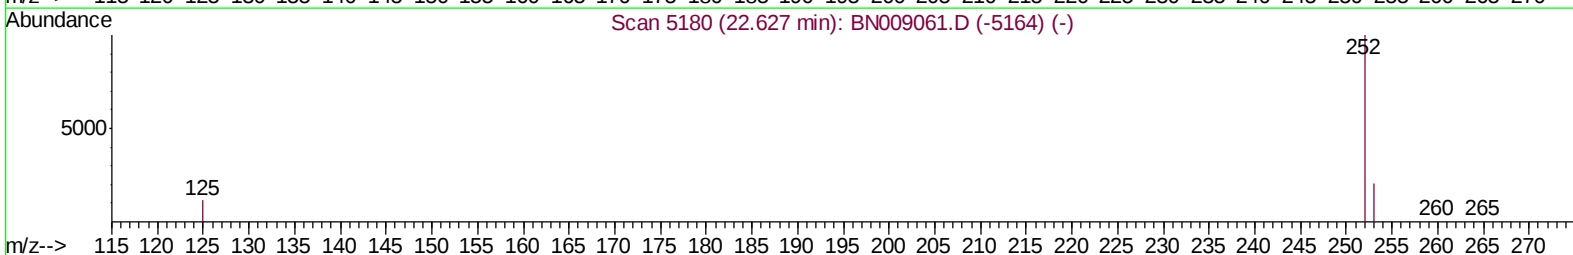
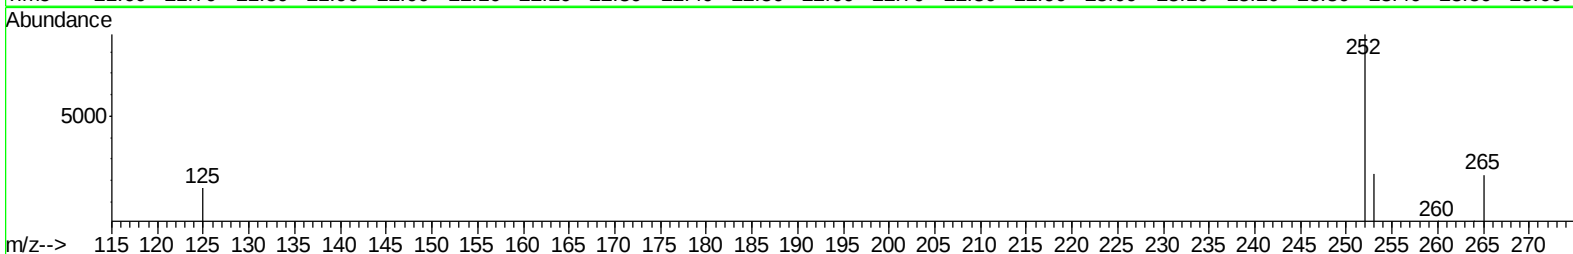


Data File : BN009075.D
Acq On : 20 Dec 2019 19:16
Operator : JU
Sample : K6171-04DL 10X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Quant Time: Dec 20 22:59:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 20 22:55:30 2019
Response via : Initial Calibration

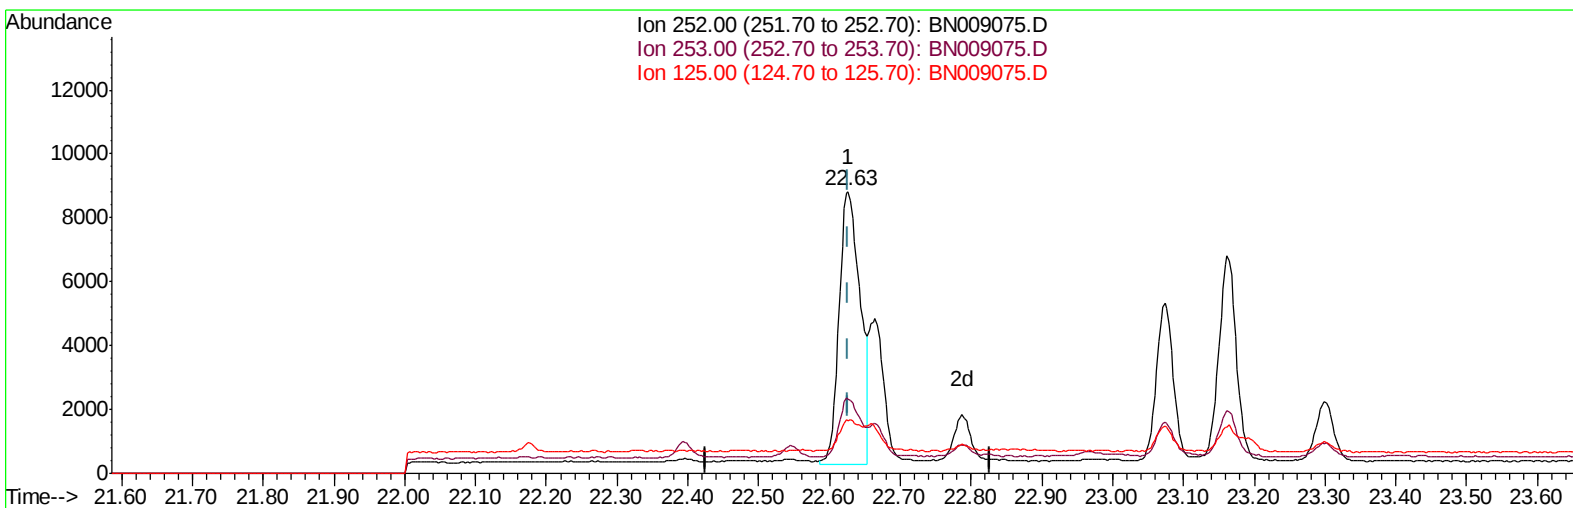

TIC: BN009075.D

(21) Benzo(b)fluoranthene

22.627min (-0.000) 0.45ng/ul m

response 17627

Ion	Exp%	Act%
252.00	100	100
253.00	24.10	26.58
125.00	15.00	18.68
0.00	0.00	0.00