
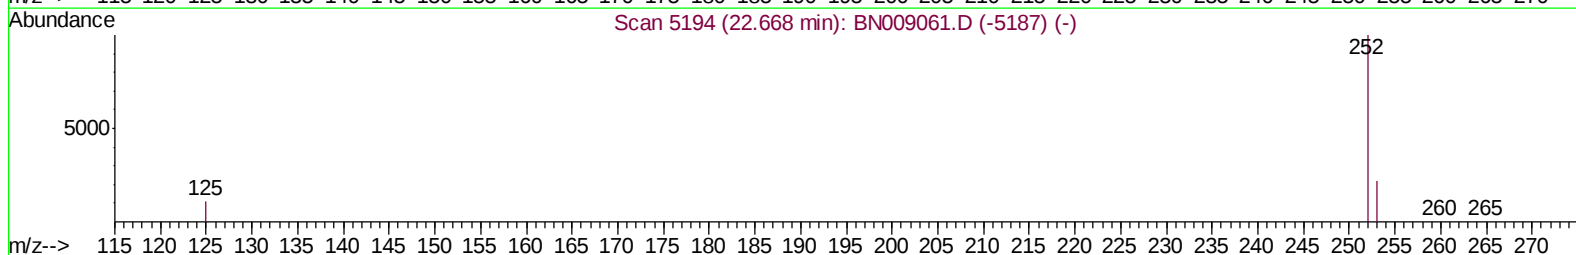
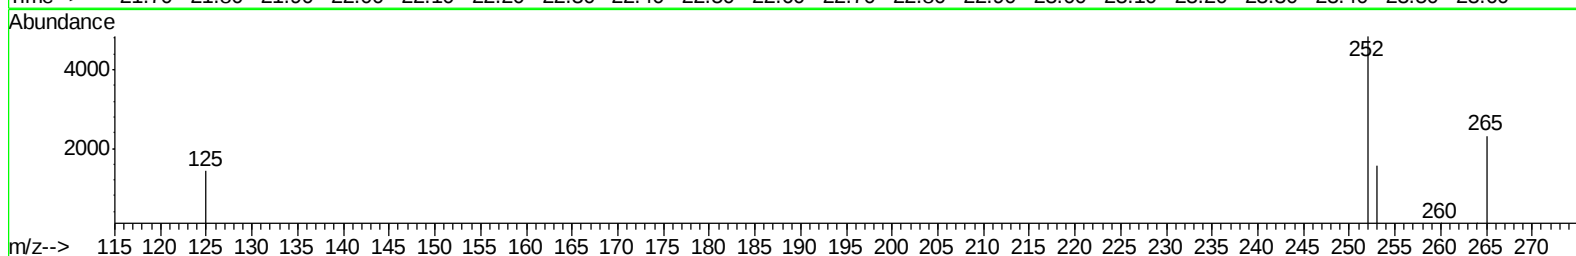


Data File : BN009075.D
Acq On : 20 Dec 2019 19:16
Operator : JU
Sample : K6171-04DL 10X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Quant Time: Dec 20 22:59:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 20 22:55:30 2019
Response via : Initial Calibration

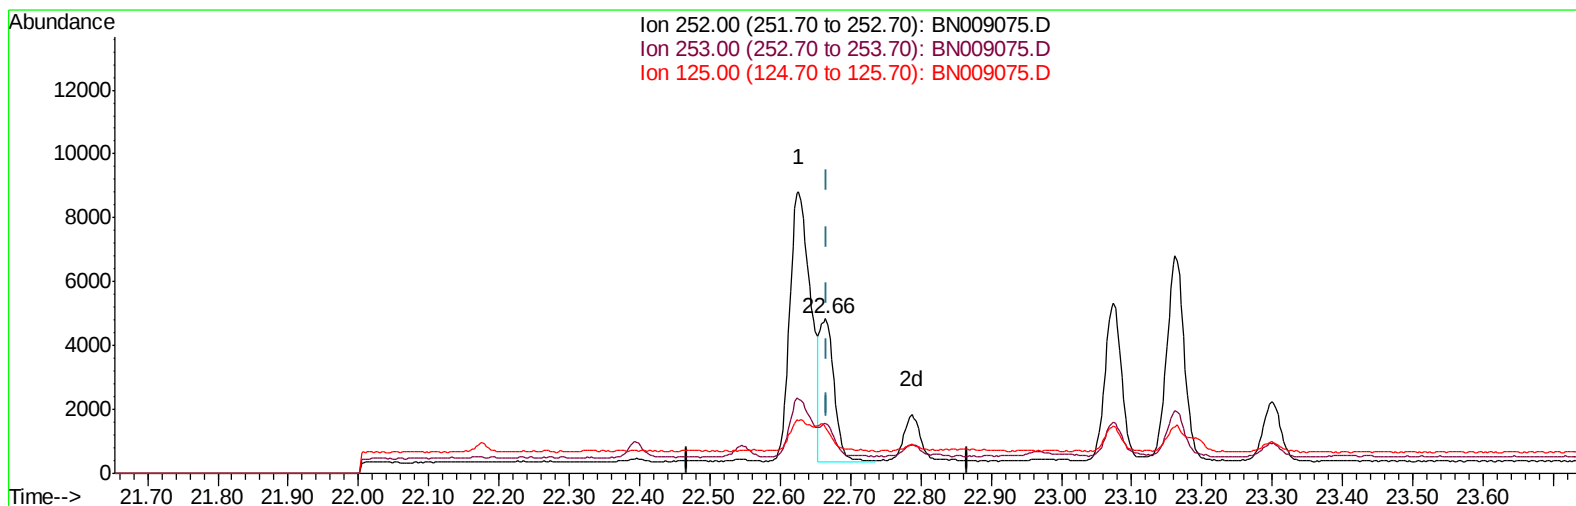

TIC: BN009075.D

(22) Benzo(k)fluoranthene

22.665min (-0.003) 0.16ng/ul m

response 6466

Ion	Exp%	Act%
252.00	100	100
253.00	24.20	32.23#
125.00	15.50	29.45#
0.00	0.00	0.00