
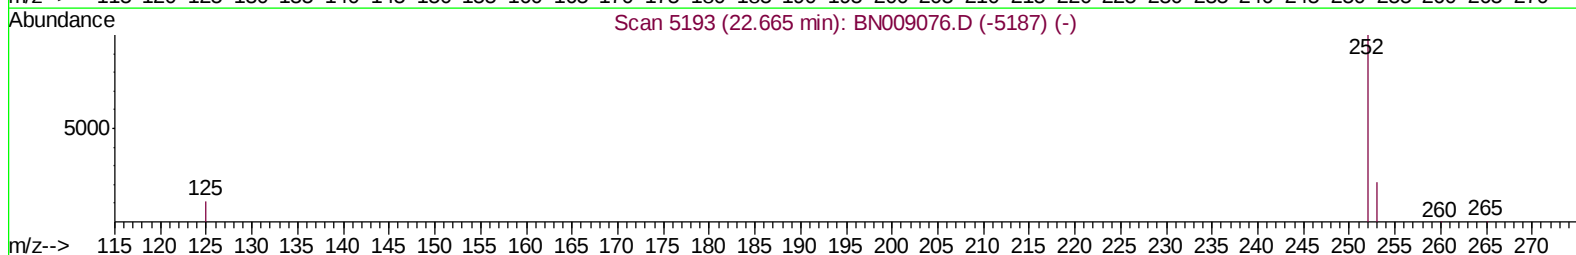
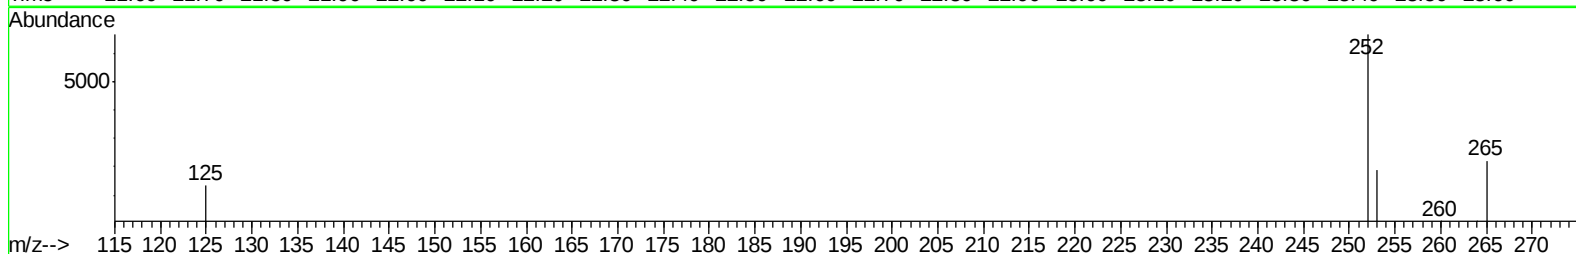


Data File : BN009077.D
Acq On : 20 Dec 2019 21:03
Operator : JU
Sample : K6171-08DL 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Quant Time: Dec 20 23:33:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 20 23:31:06 2019
Response via : Initial Calibration

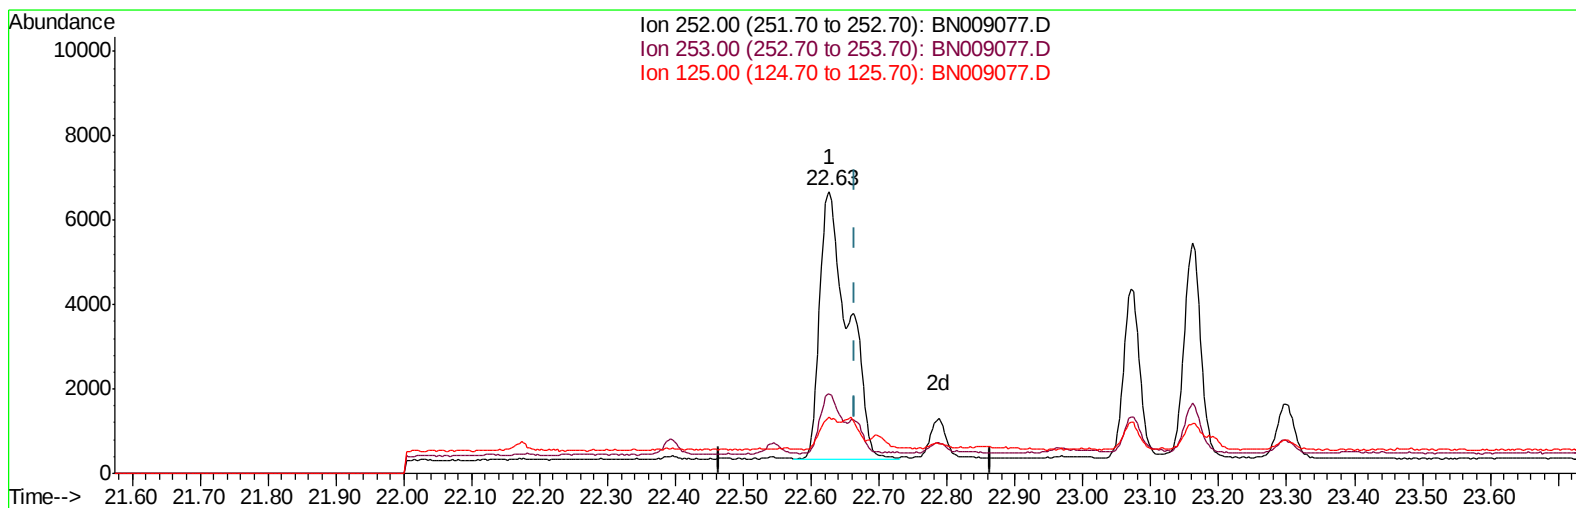

TIC: BN009077.D

(22) Benzo(k)fluoranthene
22.627min (-0.038) 0.48ng/ul
response 18349

Ion	Exp%	Act%
252.00	100	100
253.00	24.20	27.99
125.00	15.50	19.87#
0.00	0.00	0.00